




BOOK OF ABSTRACTS

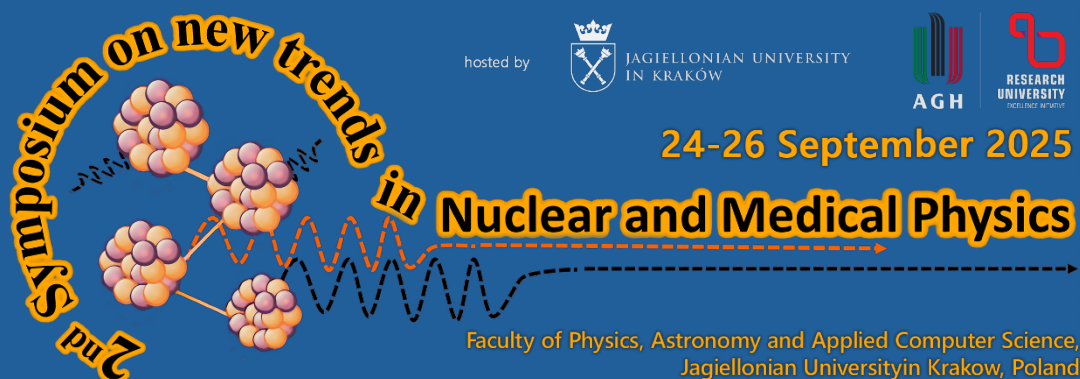

Abstract list

1	The ^{103}Pd and ^{109}Pd Bisphosphonate Complexes for Auger Electron Therapy of Bone Metastatic Tumor Cells	6
2	Constraining CP Violation in Ortho-Positronium Decays at 7 Tesla with NeuroSphere PET Modules	7
3	SiPM Performance Characterization for Total-Body J-PET: Hamamatsu vs. Onsemi	8
4	Cryo-TEM and Python-Driven 3D Reconstruction of breast cancer-derived extracellular vesicles for radiopharmaceutical characterization	9
5	Fluorescence-Guided Analysis of EV Behavior in 3D Breast Cancer Spheroids: Toward PET-Compatible Theranostics	11
6	Radiation Damage Monitoring in the Upgraded VELO Detector at LHCb	13
7	Modern Data Correction Approaches in Positron Emission Tomography	14
8	Developing efficiency maps for double isotope studies with J-PET	15
9	Treatment and online PET imaging of a mouse tumor with radioactive ion beams	16
10	In vivo radiation sensing using phase-change ultrasound contrast agents	17
11	30th anniversary of the Heavy Ion Laboratory of the University of Warsaw and its contribution to the production of medical radioisotopes	19
12	New precision limits on CPT symmetry test in positronium with J-PET	20
13	Graph-based event reconstruction for segmented detectors: SiFi-CM case study	21
14	Cd(Zn)Te in Medical Imaging: Academic Innovation and Market Transformation	22
15	Preclinical Ac-225 Imaging for Targeted Alpha Therapy: Accelerating Cancer Therapeutics	23
16	First experimental demonstration of positronium lifetime imaging with the novel radionuclide ^{52}Mn using J-PET scanner	24
17	Application of Positron Annihilation Lifetime Spectroscopy in Polymer Composites	26
18	Time-Based Separation of Scattering and Capture Processes in NAA Based on Monte Carlo Simulations in Geant4 toolkit	27
19	Developing analysis criteria for studies of CP symmetry with photons from o-Ps decay and Compton scattering with the Modular J-PET Detector	28

20	Miniature Scintillating Detectors and SiPMs: a brief Summary and a few Applications	29
21	Direct imaging of the three-photon annihilation process beyond PET	30
22	Decay Law of Selected Fluorescent Substances	31
23	Characterization of new SiC detectors for further experiments with exotic nuclei at barrier energies	32
24	Perspectives on Preclinical Molecular Imaging Research at the Radiopharmacy Centre, Medical University of Bialystok	33
25	Impact of the Midkine expression on the uptake of [18F]FDG and [18F]FET in chicken chorioallantoic membrane glioblastoma models	34
26	Automated Simulation Workflow for 3D-Printed Scintillator Phantoms in Radiotherapy Planning	36
27	Study of Total-Body J-PET sensitivity as a function of the Ring Number	38
28	First Laboratory Tests of the SABAT Project Sensor with a D-T Neutron Generator	39
29	Plan-Guided Super-Resolution of Dose Distribution	40
30	Design and construction of Cross-Staged Gantry System of Total-Body J-PET/CT Scanner for Motion Artifact Free anatomic and metabolic imaging	41
31	Optical properties and time-of-flight resolution of plastic scintillators for the total-body J-PET scanner	42
32	Can decay gammas from radioactive ion beams enhance prompt gamma imaging?	43
33	Simulated Signal Database for Improved Resolution in Position Sensitive Planar Germanium Detector	44
34	Titanium-Scandium Radionuclide Generator: A New Approach for Sustainable Isotope Production	45
35	MERMAID – prototype PET scanner for small aquatic animals	46
36	Silicon as beam-activated tumour tracer for online proton therapy monitoring – experimental study	47
37	Fragmentation measurements for particle therapy with the FOOT experiment	48
38	Usage of DL-based portal dose images for treatment error detection with transit dosimetry in radiotherapy	49
39	Normalisation Strategies in ToF-SIMS Analysis of Liver Tissue – Critical Impact on Comparative Molecular Profiling in a Diabetic Rat Model	50

40	Ex-Vivo Positronium Lifetime Imaging with ^{44}Sc Using J-PET Scanner	51
41	Measuring the degree of entanglement in matter using a plastic-scintillator based PET scanner	53
42	Nanobrachytherapy of Triple-Negative Breast Cancer and Glioblastoma Multiforme Using Auger Emitters	55
43	High Precision X-ray Spectroscopy: from Kaonic Atoms to Societal Applications	57
44	Preliminary tests of positronium gathering in microcavities connected to nanochannels	58
45	Development of a high-quality, energy-tunable positronium beam via photodetachment of positronium negative ions	60
46	In-beam PET monitoring during radioactive ion beams irradiation for realtime dose discrepancies and anatomical change detection	61
47	Quantification of Nanoscale Free Volumes in Human Plasma Clots Using Positron Annihilation Lifetime Spectroscopy	62
48	Towards feasibility study of Positronium yield in proton beam therapy	64
49	Mirror matter: towards precise measurement of orthopositronium lifetime	65
50	Prospects for Positronium and Quantum Entanglement Imaging with J-PET	66
51	Enhancement of Biological PET Imaging via Quantum Entanglement using GAGG-SiPM pixel ring detectors	67
52	Range Monitoring in Proton Therapy Using the J-PET Scanner: First Experimental Insights	68
53	Targeted radioligand therapy	69
54	Probing nuclear structure using lifetime measurements	70
55	Towards the development of an iterative algorithm for positronium lifetime imaging using ^{44}Sc with the modular J-PET	71
56	Feasibility study of Antihydrogen vertex imaging using the modular J-PET	73
57	Development of Advanced PET Technology for Scientific and Clinical Applications	75
58	Para-positronium and beyond: probing two-photon annihilation in bound states	76
59	Extracellular vesicle flow cytometry: what's possible and what's next	77

60	μ PPET, a J-PET application for cosmic rays investigation	78
61	Cold Neutron Interferometry for Fundamental Physics Experiments	79
62	Development of high-Z organic scintillators for modern SPECT imaging and theranostic dosimetry	80
63	High-Resolution Intravital Imaging: Novel On-Chip PET and iQID Camera for Personalized Radiopharmaceutical Therapy and Microdosimetry	82
64	Optimizing the event selection of the total-body J-PET scanner with a brain PET insert: a simulation study	83
65	Characterization of optical photon transport in Long Plastic Scintillators	84
66	Direct three gamma positronium imaging and cascade gamma chemical imaging	85
67	Scientific Computing: Remote Access, CNN Segmentation, and SARS-CoV2 Dynamics	86
68	Lipid Remodelling in Extracellular Vesicles from β -Cells under Hyperglycemic Stress – Multimodal Mass Spectrometry Approach	87
69	Studies of the absorption parameter $3/2$ in positronium decays	89
70	Proton-induced nuclear reactions in the hadrontherapy energy range	90
71	Extracellular Vesicles and How to Find Them	91
72	Theoretical untangling of photon entanglement detection in positronium annihilation processes	92
73	EVs as a non-invasive approach to diagnose and monitor metabolic diseases	93
74	A Geant 4 simulation of the positronium target cloud in the GBAR experiment	94
75	Search for η' -mesic nuclei with (p,dp) reaction at GSI/FAIR	95
76	Towards Charge conjugation symmetry test in Electromagnetic Interaction using J-PET	96
77	A Feasibility Study of Using Detector-Scattered Photons for Attenuation Map Generation in J-PET Scanner	97
78	Development of a millifluidic platform for slow positron beam studies of biological samples	99

1. The ^{103}Pd and ^{109}Pd Bisphosphonate Complexes for Auger Electron Therapy of Bone Metastatic Tumor Cells

Geeva Prasanth Annamalaisamy¹, Monika Lyczko¹, Aleksander Bilewicz¹

Institute of Nuclear Chemistry and Technology, Warsaw, Poland

Palladium radioisotopes ^{103}Pd and ^{109}Pd emit Auger electrons, which are known for their high linear energy transfer (LET) and ability to induce lethal damage in malignant cells at the subcellular level. These properties make them promising candidates for targeted radiotherapeutic applications.

For application of these radionuclides in bone cancer therapy, we synthesized ^{103}Pd and ^{109}Pd complexes containing one alendronate molecule and two bipyridyl ligands. The resulting compounds exhibited high stability and strong binding affinity toward hydroxyapatite, the primary inorganic component of bone tissue.


In comparative cytotoxicity assays, these radioactive complexes demonstrated higher cytotoxic effects against human prostate cancer cells (DU 145) and HER2-positive ovarian cancer cells (SKOV-3) than both ^{125}I -labeled trastuzumab (an established Auger emitter conjugate) and cisplatin.

The biological evaluation revealed that ^{103}Pd (Auger emitter) and ^{109}Pd (dual beta and Auger emitter) display pronounced cytotoxicity. It was also observed that, following the decay of ^{109}Pd , the decay product $^{109\text{m}}\text{Ag}$ dissociates from the complex. In contrast, the decay product of ^{103}Pd , $^{103\text{m}}\text{Rh}$, remains bound within the complex. This retention is likely due to the stabilizing influence of the delocalized electron system in the aromatic bipyridyl ligands, which hinders the release of $^{103\text{m}}\text{Rh}$.

These findings support the feasibility of employing the $^{109}\text{Pd}/^{109\text{m}}\text{Ag}$ and $^{103}\text{Pd}/^{103\text{m}}\text{Rh}$ pairs as in situ generators for radiotherapeutic applications and justify further investigation of this strategy in preclinical models.

This project was funded by the National Science Center Poland, grant no. 2022/45/B/ST4/00825.

The radionuclide ^{103}Pd was produced as part of the European Medical Isotope Program: PRISMAP.

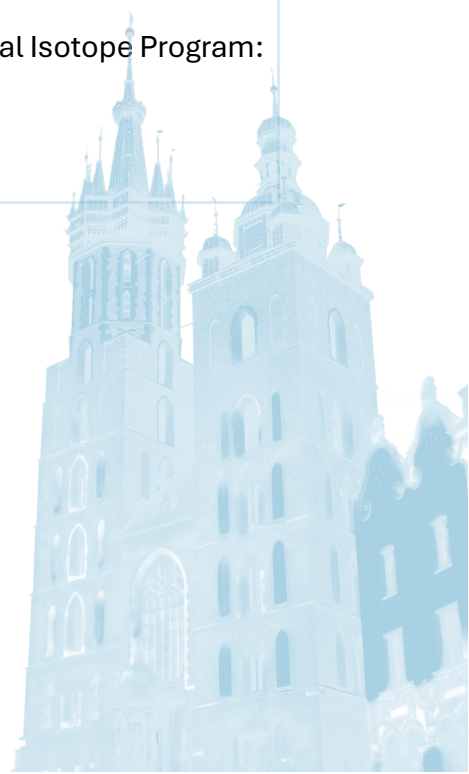

2. Constraining CP Violation in Ortho-Positronium Decays at 7 Tesla with NeuroSphere PET Modules

Magdalena S. Allen^{1,2}, Caio Silva², Michele Scipioni¹, Maryam Hiradfar¹, Or Hen², Ciprian Catana¹

¹*A. A. Martinos Center, Department of Radiology, Massachusetts General Hospital and Harvard Medical School, USA*

²*Department of Physics, Massachusetts Institute of Technology*

The decay properties of ortho-positronium (o-Ps), a bound state of a positron and an electron that can form prior to annihilation, serve as a probe of material properties (e.g., differentiating porosity or tissue pathology) and fundamental physics (e.g., testing quantum electrodynamics theory or constraining fundamental symmetry violation). In this work, we demonstrate the capability of the NeuroSphere MR-compatible PET modules to measure the o-Ps $\rightarrow 3\gamma$ decay lifetime and kinematics under an applied 7-T magnetic field. A target comprised a Na-22 positron source was placed between two slabs of polyvinyltoluene (PVT), which serve both as the formation region for o-Ps and positron emission time trigger. The target was positioned at the center of a ring of 20 NeuroSphere PET detectors (pixelated LSO arrays coupled to silicon photomultipliers), and the system was mounted on a motorized turntable at isocenter of the 7-T MRI base field for data acquisition. The long-lived component of the o-Ps decay lifetime in PVT was measured to be 31.2 ns. The measured asymmetry in o-Ps decays under the effective reversal of the magnetic field direction, as a function of the angle between the most energetic decay photon and o-Ps spin polarization axis, was measured to be 0.0102 ± 0.0100 , consistent with zero asymmetry (no CP violation).



3. SiPM Performance Characterization for Total-Body J-PET: Hamamatsu vs. Onsemi

Keyvan Tayefi Ardebili^{1,2}, Szymon Niedźwiecki^{1,2}, Pawel Moskal^{1,2}

¹*Faculty of Physics, Astronomy and Applied Computer Science, Jagiellonian University, Cracow, Poland.*

²*Center for Theranostics, Jagiellonian University, Cracow, Poland.*

Total-body Positron Emission Tomography (PET) has begun to see clinical use; however, widespread adoption in hospitals requires a significant reduction in construction costs [1]. We are developing a cost-effective total-body J-PET system based on plastic scintillator strips coupled with Silicon Photomultipliers (SiPMs) at their axial ends [2]. A critical aspect of optimizing this involves the comparison of different SiPM types. SiPMs, representing the latest generation of photomultipliers, offer significant advantages over traditional Photomultiplier Tubes (PMTs) [3], including low operating voltage and insensitivity to magnetic fields, making them ideal for various applications, including nuclear medicine. This study focuses on characterizing and comparing the performance of different SiPM types from leading manufacturers, Hamamatsu and Onsemi, to identify the optimal SiPM for the total-body J-PET system. In the experimental phase, individual detector units comprising plastic scintillator strips ($6 \times 6 \times 25$ mm³) coupled with Hamamatsu (S14160-6050HS) and Onsemi (MICROFJ-60035-TSV) SiPMs of identical active surface area were thoroughly characterized. A collimated beam of 511 keV photons from a Na-22 isotope source was employed to evaluate key detector performance parameters, including signal amplitude, rise time, fall time, charge, and Time of Flight (TOF) resolution [4]. Following this thorough characterization and comparative analysis, the optimal SiPM was identified for integration into the total-body J-PET system, contributing to its cost-effective and high-performance design.

[1] P. Moskal, E. Stępień, PET Clin. 15, 439-452, 2020

[2] P. Moskal et al., Phys. Med. Biol. 66, 175015, 2021

[3] S. Niedźwiecki et al., Acta Phys. Polon. B 48, 1567, 2017

[4] P. Moskal et al., Nucl. Instrum. Meth. A 764, 317-321, 2014



4. Cryo-TEM and Python-Driven 3D Reconstruction of breast cancer-derived extracellular vesicles for radiopharmaceutical characterization

Kriti Awasthi^{1,2}, Narendra Rathod³, Magdalena Kostkiewicz⁴ and Ewa Stepień^{1,2}

¹*Faculty of Physics, Astronomy and Applied Computer Science, Jagiellonian University, Cracow, Poland.*

²*Center for Theranostics, Jagiellonian University, Cracow, Poland*

³*University of Bern, Bern, Switzerland.*

⁴*Department of Cardiovascular Diseases, Collegium Medicum Jagiellonian University, Department of Nuclear Medicine Hospital John Paul II, Cracow, Poland*

Extracellular vesicles are upcoming versatile nano-carriers for the use in diagnosis and therapeutic delivery in the oncological studies. In triple negative breast cancer (TNBC), EVs secreted by MDA-MB-231 cells are specifically designated to use for radiopharmaceutical applications due to their intrinsic tumour tropism and biocompatibility. However, their functional usage in nuclear medicine needs to be discovered and unveiled, which requires a deeper understanding of their nanoscale morphology and its surface architecture, which impacts the radionuclide labelling, stability and targeting efficiency. In this research, we employed cryo-TEM images combined with a custom Python-based computational pipeline to perform 3D tomographic reconstructions of MDA-MB-231 derived EVs. The EVs were isolated via differential ultracentrifugation and used for high-resolution cryo-TEM imaging. The tilt series arrangements were processed using IMOD and 3D reconstruction, segmentation and rendering were processed using python tools which includes NumPy, scikit-learn image and pyTom. These reconstructions reveal diverse morphologies ranging from single membrane and multivesicular forms to membrane protrusions and internal cargo compartments features critical for understanding vesicle behaviour in vivo. The characterisation of potential radiolabelling sites and evaluated surface geometry relevant for conjugating PET/SPECT tracers was also studied. This consolidative approach provides a structural foundation for optimizing EV-based radiopharmaceutical workflow. By using open source python tools for tomographic analysis, this workflow allows reproducible and high resolution EV characterisation which is important for advancing precision imaging and targeted radiotherapy in the field of oncology.

Acknowledgements :

The research was financed by the Polish agency National Science Center as part of the OPUS project for E.S. (2022/45/B/NZ7/01430)

The CRYO-TEM part was conducted under the provision of the Polish Ministry and Higher Education project Support for research and development with the use of

research infrastructure of the National Synchrotron Radiation Centre SOLARIS” under contract nr 1/SOL/2021/2. We acknowledge the SOLARIS Centre for access to the cryogenic electron microscope, where the measurements were performed.



5. Fluorescence-Guided Analysis of EV Behavior in 3D Breast Cancer Spheroids: Toward PET-Compatible Theranostics

Kriti Awasthi^{1,2}, Magdalena Kostkiewicz³, Maciej Słotwiński^{1,2} and Ewa Stepień^{1,2}

¹Faculty of Physics, Astronomy and Applied Computer Science, Jagiellonian University, Cracow, Poland.

²Center for Theranostics, Jagiellonian University, Cracow, Poland

³Department of Cardiovascular Diseases, Collegium Medicum Jagiellonian University, Department of Nuclear Medicine Hospital John Paul II, Cracow, Poland

To study the characteristics of in-vivo tumours with respect to its cellular heterogeneity and their spatial architecture, the most impactful approach will be three-dimensional (3D) tumor modeling of spheroids, which is a powerful alternative to existing traditional 2D monolayer models. With respect to triple-negative breast cancer (TNBC), as per the disease's aggressiveness and limited treatment options these models are valued. In this research, we utilised GFP-expressing MDA-MB-231 cells to generate reproducible 3D spheroids for investigating naturally secreted extracellular vesicles (EVs). EVs are versatile and play an important role in intercellular communication and recently highlighted both as biomarkers and potential carriers in precision oncology. Our model allows real time fluorescence based imaging of EV uptake and distribution within spheroid layers, eliminating the need for artificial dye labelling and preserving EVs integrity. The major highlight of this project is the comparative profiling of EVs derived from 2D versus 3D cultures, with focusing on identifying the dimensionality which can influence EV production and surface markers. Importantly, this model also provides a platform for the future integration of radiopharmaceuticals, specifically for PET based tracking and theranostic applications. By enhancing imaging workflows with physiological relevance to the microenvironment, this study paves the way for EV based radiotracer development in oncology. Our results depict the utility of 3D spheroid systems in EV research and carve their translational potential for future radiopharmaceutical imaging and delivery schemes in cancer biology.

Acknowledgements :

The research was financed by the Polish agency National Science Center as part of the OPUS project for E.S. (2022/45/B/NZ7/01430)

The research was financially supported by the Research Support Module 1 in the Strategic Programme Excellence Initiative at Jagiellonian University, 2025. ID: RSM/109/AK



6. Radiation Damage Monitoring in the Upgraded VELO Detector at LHCb

Saliha Bashir, Tomasz Szumlak, Agnieszka Oblakowska-Mucha

AGH University of Science and Technology, Cracow, Poland

The upgraded VELO (Vertex LOcator) is a lightweight hybrid pixel silicon vertex detector that surrounds the interaction region of the LHCb experiment. It plays a critical role in the precise reconstruction of both primary and secondary vertices. Silicon-based semiconductor detectors are well-suited for this purpose, offering high spatial resolution, fast response times, and the ability to handle high interaction rates.

However, the intense radiation environment of the Large Hadron Collider (LHC) poses a significant challenge to the longevity of silicon sensors. Radiation-induced damage—including increased leakage current, charge trapping, and shifts in depletion voltage—progressively degrades detector performance. Accurate understanding and quantification of this damage are essential for optimizing current detector performance and guiding the design of future upgrades.

This work focuses on radiation damage monitoring in the upgraded VELO detector. A data-driven study of particle fluence is presented to characterize the radiation environment during LHC operation. By correlating fluence estimates with observed changes in detector behaviour, this study aims to refine predictive models of radiation damage and contribute to the development of robust long-term operational strategies for silicon vertex detectors.



7. Modern Data Correction Approaches in Positron Emission Tomography

Reimund Bayerlein

University of California Davis, USA

Positron Emission Tomography (PET) is a powerful molecular imaging modality widely used in oncology, neurology, and cardiology. However, the accuracy and diagnostic value of PET images depend heavily on the application of robust data correction techniques. In hybrid PET/CT and PET/MR systems, attenuation correction (AC), scatter correction (SC), and motion correction (MC) are essential to mitigate various physical effects that compromise image quality and quantitative accuracy.

Attenuation correction addresses the reduction of photon intensity due to tissue absorption, a critical factor for accurate tracer quantification. Scatter correction compensates for Compton-scattered photons that otherwise introduce image blurring and quantitative bias. Motion correction targets patient motion – caused by respiration, cardiac activity, voluntary movement, or physiological processes – aiming to restore lesion sharpness and improve quantification across the extended duration of PET acquisitions.

The presentation will highlight recent advances in each correction category, driven by innovations in instrumentation, detector materials, scanner geometries, and clinical demands. We will cover both classical analytical methods and emerging deep learning-based approaches, emphasizing their theoretical foundations, practical implementations, and comparative effectiveness in modern PET workflows.



8. Developing efficiency maps for double isotope studies with J-PET

E. Y. Beyene^{1,2}, P. Moskal^{1,2}, E. Stepień^{1,2} for the J-PET Collaboration

¹*Faculty of Physics, Astronomy and Applied Computer Science, Jagiellonian University, Cracow, Poland.*

²*Center for Theranostics, Jagiellonian University, Cracow, Poland.*

The study is aimed at developing efficiency maps for both two-photons (2γ) as well as two-photons and prompt gamma ($2\gamma + \gamma_P$) detection modes for the simultaneous double isotope studies using the modular prototype Jagiellonian Positron Emission Tomography (J-PET) scanner [1, 2]. Simulations were performed using Gate 9.4 modeling back-to-back 511 keV annihilation photons and 1275 keV prompt gammas from ^{22}Na source.

A uniform cylinder volume source (radius = 18.475 cm) was simulated for the 2γ and $2\gamma + \gamma_P$ cases. For representing a continuous ^{22}Na source, events were registered in the 3D grid of $2.5 \text{ mm} \times 2.5 \text{ mm} \times 2.5 \text{ mm}$ voxel width. The candidates of 2γ and $2\gamma + \gamma_P$ events were selected based on the energy loss, time and positions of interactions [1, 3]. The Efficiency maps were plotted using Cartesian coordinates and also transformed into polar coordinates aligned with the cylindrical geometry of the scanner. Additionally, absolute efficiency line profiles were evaluated for both prompt and 511 keV using the single photon emission model, with comparisons made to experimental measurements.

The acquired profiles and maps reveal performance differences between the two types of events and efficiencies, providing insight into how image reconstruction, analysis, and separation can be improved in modular J-PET systems for double isotope studies using pure β^+ and $\beta^+ + \gamma_P$ emitting isotopes [1].

[1] E. Beyene et al., Bio-Algorithms Med-Syst., vol. 19, p. 101, 2023.

[2] P. Moskal et al., Sci. Adv., vol. 7, p. eabh4394, 2021.

[3] P. Moskal et al., Sci. Adv., vol. 10, p. eadp2840, 2024.



9. Treatment and online PET imaging of a mouse tumor with radioactive ion beams

Daria Boscolo¹, Giulio Lovatti², Olga Sokol¹, Tamara Vitachio¹, Martina Moglioni¹, Francesco Evangelista², Emma Haettner¹, Walter Tinganelli¹, Christian Graeff¹, Uli Weber¹, Christoph Schuy¹, Munetaka Nitta², Daria Kostyleva¹, Sivaji Purushothaman¹, Peter Thierolf², Jonathan Bortfeldt², Katia Parodi², Marco Durante¹, Christoph Scheidnberger¹


¹*GSI Helmholtz Centre for Heavy Ion Research, Darmstadt, Germany*

²*Ludwig-Maximilians-Universität München, LMU, Munich, Germany*

While charged particle therapy is potentially the most effective radiotherapy technique available, it is highly susceptible to range uncertainties. Radioactive ion beams (RIBs) have long been proposed for therapy applications, offering the potential for image-guided treatment through positron emission tomography (PET). In this contribution, we will present the results of the first preclinical study using ¹¹C ion beams combined with real-time PET imaging. The study investigated whether RIB could provide precise tumor control while minimizing toxicity to organs-at-risk (OAR) [1].

In particular, ¹¹C-ion beams were produced via in-flight separation, characterized, and precisely modulated to treat synergetic tumors implanted in the mouse neck area. The tumors were close to the spinal cord, increasing the risk of radiation-induced myelopathy. Mice were treated with a single dose application of 5 Gy or 20 Gy, and all the irradiations were imaged in real-time using a custom-built PET scanner. Tumor growth, spinal cord toxicity, and PET-based activity were evaluated. Complete tumor control was obtained with the highest dose. Low-grade neurological side effects were correlated to the positron activity measured in the spine. Additionally, a dose dependent biological washout of the PET signal was observed, indicating a potential component of vascular damage at high doses. This experiment marks the first instance of tumor treatment using RIB and paves the way for future clinical applications.

[1] D. Boscolo et al., First image-guided treatment of a mouse tumor with radioactive ion beams, submitted. [Online]. Available: <https://doi.org/10.48550/arXiv.2409.14898>

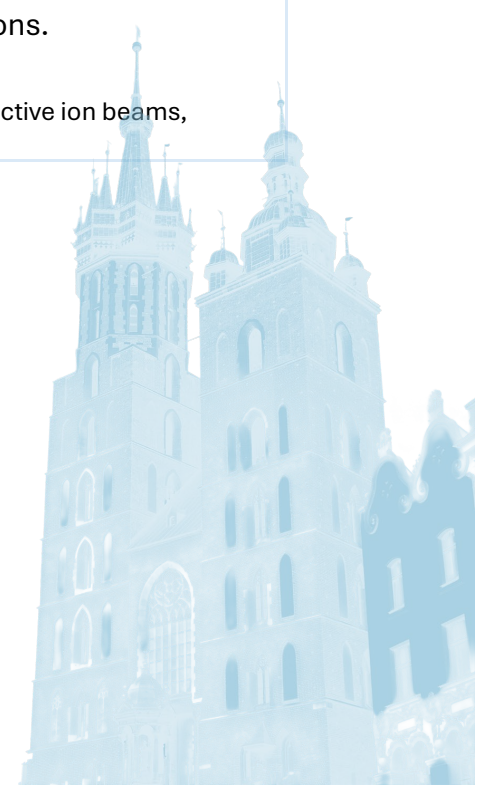

10. In vivo radiation sensing using phase-change ultrasound contrast agents

Bram Carlier¹, Edmond Sterpin¹, Uwe Himmelreich¹

¹KU Leuven, Belgium

Radiotherapy is one of the most effective cancer treatment strategies, able to benefit up to 50% of the cancer patients [1]. In the majority of treatments, external photon beam radiotherapy is used. Yet, photons feature unfavourable depth-dose characteristics resulting in undesired exposure of healthy tissue. Therefore, proton therapy has emerged as a promising alternative. Owing to the Bragg peak, the proton dose can be accumulated precisely in the tumour, with minimal damage to healthy tissue. Nevertheless, the sharp dose gradients associated with proton treatments, make them sensitive to uncertainties, e.g. induced by the conversion of CT HU to proton stopping powers, patient setup errors, patient motion or anatomical changes throughout the treatment [2]. While they are accounted for during treatment planning, e.g. by using margins around the tumour, the resulting (often overly conservative) treatment plans again increase exposure risks to healthy tissue and less efficient irradiation of the tumour, obscuring the true benefits of proton therapy.

Therefore, uncertainties are ideally reduced by using *in vivo* dosimetry or range verification technologies. Nevertheless, despite decades of research giving rise to technologies like PETbased range verification, prompt gamma imaging and ionoacoustics, none of the proposed approaches have entered standard clinical practice due to various limitations including poor resolution, indirect relationship to the proton range, complex detector development or weak signals [2–4].

To overcome these limitations, we proposed an alternative method for *in vivo* radiation sensing based on radiation-sensitive phase-change ultrasound contrast agents. In particular, we developed superheated nanodroplets, which can be converted into echogenic microbubbles upon proton irradiation [5–7]. The radiation deposition is subsequently derived from the resulting ultrasound contrast. In a first phase, we demonstrated the submillimetre range retrieval performance of the proposed technology in nanodroplet-containing gel phantoms [5–7]. Afterwards, we confirmed the biocompatibility of the used contrast agents *in vitro*, and confirmed the dose and energy dependent radiation response *in vivo*, in the liver of healthy rats [8]. Finally, we are also developing computational prediction models able to convert the original treatment plan into a predicted vaporization map. This way a clinician simply needs to compare the observed and predicted response to determine whether the treatment was indeed delivered as intended.

Together these results form a convincing foundation to promote clinical translation and pave the way for alternative applications, like radiation-induced drug delivery employing these radiation-sensitive contrast agents as theranostic drug delivery vehicles.

- [1] Y. Lievens, J. M. Borras, and C. Grau, *Mol. Oncol.*, vol. 14, pp. 1461–1469, 2020
- [2] A. C. Knopf and A. Lomax, *Phys. Med. Biol.*, vol. 58, pp. 131–160, 2013
- [3] K. Parodi, *Br. J. Radiol.*, vol. 93, p. 20190590, 2020.
- [4] W. Assmann et al., *Med. Phys.*, vol. 42, pp. 567–574, 2015
- [5] B. Carlier et al., *Phys. Med. Biol.*, vol. 65, p. 065013, 2020
- [6] S. V. Heymans et al., *Med. Phys.*, vol. 48, pp. 1983–1995, 2021
- [7] G. Collado-Lara et al., *Ultrasound Med. Biol.*, vol. 48, pp. 149–156, 2022
- [8] B. Carlier et al., *Phys. Med. Biol.*, vol. 69, p. 205014, 2024



11. 30th anniversary of the Heavy Ion Laboratory of the University of Warsaw and its contribution to the production of medical radioisotopes

Jarosław Choiński

Heavy Ion Laboratory, University of Warsaw, Poland

In 2024, the Heavy Ion Laboratory of the University of Warsaw (HIL) celebrated its 30th anniversary. When designing the Laboratory building, one of the boxes was designated for an installation dedicated to the production of radioisotopes using U-200P heavy ion cyclotron beams. The presentation will provide a brief history of the HIL construction. The team's involvement in the production of radioisotopes obtained in heavy ion nuclear reactions will be emphasized. The history of HIL's expansion to include the Radiopharmaceutical Production and Research Center (RPRC) will also be discussed. The center houses the PETtrace cyclotron, which allows for the acceleration of protons or deuterons. In the course of implementing two research projects: "Alternative Methods for the ^{99m}Tc Production" Agreement No PBS1/A9/2/2012 funded by the National Centre for Research and Development and "The development of methods for production of new radiopharmaceuticals based on Sc radionuclides used in positron tomography (PET)" [PET-SKAND] agreement no PBS3/A9/28/2015 awarded to a consortium, and financed by the National Centre for Research and Development, an external stand for irradiation of solid targets in metallic or powder form was built at the RPRC. Having such an experimental setup in Poland allowed HIL to enter a joint program implemented by the Jagiellonian University, the Institute of Nuclear Chemistry and Technology and HIL called Development of three-photon emitting radiotracers for positronium imaging, agreement no UMO-2021/43/B/ST2/02150, financed by the National Science Centre.



12. New precision limits on CPT symmetry test in positronium with J-PET

Neha Chug^{1,2} and Paweł Moskal^{1,2}

¹Faculty of Physics, Astronomy and Applied Computer Science, Jagiellonian University, Cracow, Poland.

²Center for Theranostics, Jagiellonian University, Cracow, Poland.

We present new results from a test of CPT symmetry in ortho-positronium (o-Ps) decays with the Jagiellonian Positron Emission Tomograph (J-PET) detector. The test investigates a CPT-odd angular correlation involving the o-Ps spin and the normal to its decay plane. J-PET is a novel technology employed to detect the multi photons from positronium annihilation [1,2]. Its high geometrical acceptance and high angular resolution of annihilation photons enable the detection of various kinematic configurations, allowing for high-precision measurements of angular correlations in o-Ps decays [3,4]. We will discuss the future perspective of increasing the sensitivity of such tests with a new J-PET prototype.

Research supported by NCN projects 2019/35/B/ST2/03562, 2021/42/A/ST2/00423 and 2022/45/N/ST2/04084.

[1] P. Moskal et al., Sci. Adv., vol. 7, p. eabh4394, 2021.

[2] P. Moskal et al., Sci. Adv., vol. 10, p. eadp2840, 2024.

[3] P. Moskal et al., Nat. Commun., vol. 12, p. 5658, 2021.

[4] P. Moskal et al., Nat. Commun., vol. 15, p. 78, 2024.



13. Graph-based event reconstruction for segmented detectors: SiFi-CM case study

Philippe Clement^{1,2}, Aleksandra Wrońska¹, Alexander Fenger², Ronja Hetzel^{2,3}, Achim Stahl², Dominik Szubartowski¹, Monika Kercz¹, Katarzyna Rusiecka¹

¹Faculty of Physics, Astronomy and Applied Computer Science, Jagiellonian University, Cracow, Poland.

²RWTH Aachen, Germany

³GSI Darmstadt, Germany

The contribution presents a newly developed approach based on Graph Neural Networks (GNN) for event reconstruction in the 1D coded-mask gamma camera for prompt-gamma imaging in proton therapy, developed within the SiFi-CC collaboration. The aim is to determine the position and energy deposit of individual gamma interactions in the detector to enable online beam range monitoring. Its sensitive part consists of scintillating LYSO fibers, read out from both sides via silicon photomultipliers (SiPMs).

The input to the GNN is formed by raw experimental data: clustered SiPM responses within 15-ns time windows. The GNN processes this cluster data – consisting of the position, timestamp, and photon count of each SiPM – as an undirected graph.

The GNN approach enables robust reconstruction of hit positions and energy even in the presence of faulty or non-functional channels, helping to bridge acceptance gaps. The goal is to improve spatial and energy resolution compared to classical methods. The model has already been integrated into the existing data processing pipeline of the research group and thus supports the evaluation of future experiments.

This contribution highlights the potential of graph-based learning methods to address detector-specific challenges in medical imaging and lays the foundation for learning-based event processing in future PGI systems.



14. Cd(Zn)Te in Medical Imaging: Academic Innovation and Market Transformation

Tuba Conka

Fraunhofer IIS, Germany

Cadmium Telluride (CdTe) and Cadmium Zinc Telluride (CdZnTe, commonly referred to as CZT) are II-VI compound semiconductors that have emerged as pivotal materials in medical imaging due to their exceptional ability to detect X-rays and gamma rays with high efficiency and energy resolution. Their high atomic numbers (Cd: 48, Te: 52, Zn: 30) and densities ($\sim 5.8\text{--}5.85\text{ g/cm}^3$) enable superior absorption compared to traditional silicon or germanium detectors, while their wide bandgaps (CdTe: 1.44 eV, CdZnTe: 1.44–2.2 eV) allow room-temperature operation, eliminating the need for cryogenic cooling. These properties make CdTe and CdZnTe ideal for advanced imaging modalities, including Single-Photon Emission Computed Tomography (SPECT), Photon-Counting Computed Tomography, and emerging applications in Positron Emission Tomography (PET). This abstract synthesizes recent academic research and market developments, to elucidate the transformative potential of CdTe and CdZnTe in medical imaging, emphasizing their material differences, current applications, and future prospects



15. Preclinical Ac-225 Imaging for Targeted Alpha Therapy: Accelerating Cancer Therapeutics

Biswajit Das^{1,2}, Jingjie Yu¹, David Goodman³, Michael Streicher³, Qihui Lyu¹,
Youngho Seo¹, Javier Caravaca^{1,2}

¹*University of California San Francisco & Lawrence Berkeley National Laboratory, USA*

²*Lawrence Berkeley National Laboratory, California, USA*

³*H3D, Inc., Ann Arbor, MI, USA*

Radiopharmaceuticals based on Actinium-225 for targeted alpha therapy (TAT) have shown encouraging results in both preclinical studies and clinical trials [1], expecting them as a promising approach for future cancer treatments [2]. In vivo imaging of small animals plays a vital role in understanding the biokinetics of 225Ac-labeled compounds and in accelerating the development and evaluation of new radiopharmaceuticals [3]. Precise imaging across a wide photon energy spectrum is essential in nuclear medicine not only for accurate diagnosis and dosimetry but also for effective monitoring of therapeutic outcomes. Although Single Photon Emission Computed Tomography (SPECT) has been the dominant technique for imaging of single gamma-emitting radionuclides over recent decades, its limited sensitivity and narrow energy range make it inadequate for imaging of therapeutic isotopes like 225Ac with broad and complex emission profiles. There remains a pressing clinical need for a high-sensitivity imaging system capable of detecting both low- and high-energy gamma rays. To address this, we propose the development of a high-sensitivity Compton imaging system and a collimated Compton camera featuring a 3D-positioning gamma-ray tracking detector [4,5]. This system is designed to enable efficient imaging of 225Ac and its decay products. At the conference, the imaging results of 225Ac daughters using these advanced imaging modalities, along with a discussion on future directions for in vivo imaging of 225Ac in small-animal models will be presented.

[1] D. A. Scheinberg and M. R. McDevitt, Curr. Radiopharm., vol. 4, no. 4, pp. 306–320, 2011.

[2] C. Parker, V. Lewington, et al., JAMA Oncol., vol. 4, pp. 1765–1772, 2018.

[3] A. P. Bidkar et al., Clin. Cancer Res., vol. 29, no. 10, pp. 1916–1928, 2023.

[4] J. Caravaca et al., IEEE Trans. Radiat. Plasma Med. Sci., vol. 6, no. 8, pp. 904–915, 2022.

[5] B. Das et al., IEEE Trans. Radiat. Plasma Med. Sci., Jun. 2025

16. First experimental demonstration of positronium lifetime imaging with the novel radionuclide ^{52}Mn using J-PET scanner

Manish Das¹, Sushil Sharma¹, Ewa Ł. Stepień¹, Paweł Moskal¹, On behalf of the J-PET collaboration

¹*Faculty of Physics, Astronomy and Applied Computer Science, Jagiellonian University, Cracow, Poland.*

²*Center for Theranostics, Jagiellonian University, Cracow, Poland.*

Positronium lifetime imaging (PLI) [1,2], an extension of PET, provides insight into the sub molecular properties of tissues by imaging the lifetime of the positronium atom [3]. Currently, the method is undergoing rapid development in terms of image reconstruction [4,5] and detection systems [6,7]. The first studies with the J-PET scanner using ^{68}Ga have demonstrated the feasibility of this technique in human subjects [6]. However, ^{68}Ga isotope has limitation mainly due to its low yield of de-excitation photons necessary for positronium lifetime estimation. In this context, ^{52}Mn emerges as a promising candidate for PLI [8], offering a half-life of 5.59 days and a cascade of three high-energy prompt photons (1434 keV, 936 keV, and 744 keV) in almost 100% cases following the positron emission, thereby increasing the sensitivity for PLI. In this work, we report the results of the successful demonstration of PLI with ^{52}Mn using the Modular J-PET tomograph, featuring triggerless data acquisition that enables simultaneous multiphoton detection [9]. ^{52}Mn was produced at the Hevesy Laboratory in Department of Health Technology at Technical University of Denmark via $^{52}\text{Cr}(p,n)^{52}\text{Mn}$ nuclear reaction and transported to Jagiellonian University in Kraków. A NEMA IQ phantom with six spheres was used for this study. The spheres were filled with ^{52}Mn , diluted in water to achieve required activity concentration. Event selection was based on the simultaneous detection of two 511 keV photons and one de-excitation photon, enabling reconstruction of images of the mean positronium lifetime [3,6]. The measured mean o-Ps lifetime shows good agreement with previously reported values in water [10]. This study presents the first-ever demonstration of PLI with ^{52}Mn , marking a significant advancement and opening new possibilities for the development of PLI for clinical applications.

Acknowledgments

This work was supported by the National Science Centre of Poland (Grants: 2021/42/A/ST2/00423, 2021/43/B/ST2/02150, 2022/47/I/NZ7/03112), SciMat and qLife under the Excellence Initiative at Jagiellonian University, PRISMAP via Project 1729020993 aniX3 and PLGrid (ACK Cyfronet AGH, PLG/2024/017688).

[1] P. Moskal, Proc. 2019 IEEE Nucl. Sci. Symp. Med. Imaging Conf. (NSS MIC), Manchester, pp. 1–3, 2019.

[2] P. Moskal et al., IEEE Trans. Radiat. Plasma Med. Sci., early access, 2025.

[3] P. Moskal et al., Sci. Adv., vol. 7, p. eabh439, 2021.

[4] B. Huang et al., IEEE Trans. Med. Imaging, vol. 43, pp. 2148–2158, 2024.

- [5] H. Huang et al., IEEE Trans. Radiat. Plasma Med. Sci., vol. 9, pp. 478–486, 2025.
- [6] P. Moskal et al., Sci. Adv., vol. 10, p. eadp2840, 2024.
- [7] W. M. Steinberger et al., EJNMMI Phys., vol. 11, p. 76, 2024.
- [8] M. Das et al., Bio-Algorithms Med. Syst., vol. 19, pp. 87–95, 2023.
- [9] P. Moskal et al., Nat. Commun., vol. 12, p. 5658, 2021.
- [10] K. Kotera et al., Phys. Lett. A, vol. 345, pp. 184–190, 2005.



17. Application of Positron Annihilation Lifetime Spectroscopy in Polymer Composites

Ewa Dryzek¹, Mirosław Wróbel²

¹*Institute of Nuclear Physics Polish Academy of Sciences, Cracow, Poland*

²*AGH University of Science and Technology, Cracow, Poland*

In biomedical applications, polymer composites are used in tissue engineering, drug delivery systems, and implant design. Generally, the wide range of performance requirements induces active, continuous development of various polymer matrix composites—including thermoplastics, thermosets, and elastomers reinforced with micro- and nano-scale fillers. The markedly different properties of these fillers compared to the polymer matrix, their tailored architectures, and their adhesion strength to the matrix contribute to the desired performance characteristics of the resulting composites. While the properties of the matrix and filler materials can usually be determined with relative ease, assessing interfacial adhesion characteristics experimentally remains a significant challenge. Positron annihilation lifetime spectroscopy (PALS) has been proposed and explored in the literature. That is because PALS is highly sensitive to nanoscale voids or free volumes between polymer chains, which strongly influence various functional properties such as electrical and thermal conductivity, mechanical performance, and gas permeability. This sensitivity makes PALS a valuable tool for characterizing polymer structures.

It has also been successfully applied to characterize polymer-based composites, e.g., [1]. Beyond measuring the size and fraction of free volume, PALS also enables the evaluation of interfacial interaction strength between composite fillers and the polymer matrix. This is done using the interfacial interaction parameter, introduced by Liu and Jean [2] for polymer blends. The parameter is conceptually analogous to the dimensionless Flory–Huggins interaction parameter, χ , which describes enthalpic contributions to mixing polymers and solvents in non-ideal solutions [3]. The use of this parameter will be reviewed. Attention was also paid to studies on the influence of filler particle size and dispersion on annihilation characteristics [4,5], and changes of the free volume structure accompanying crack initiation and propagation in tensile tests in fiber reinforced polymers [6,7].

[1] M. Luo, F. Wei, C. Jiang, J. H. Zhang, W. Xu, J. D. Liu, B. J. Ye, and H. J. Zhang, *Polymer*, vol. 320, p. 128076, 2025.

[2] J. Liu and Y. C. Jean, *Macromolecules*, vol. 28, pp. 5774–5779, 1995.

[3] M. L. Huggins, *J. Am. Chem. Soc.*, vol. 64, pp. 1712–1719, 1942.

[4] P. Winberg, M. Eldrup, and F. H. J. Maurer, *Polymer*, vol. 45, pp. 8253–8264, 2004.

[5] D. Bieliński, L. Ślusarski, O. Dobrowolski, P. Głąb, and E. Dryzek, *Kautsch. Gummi Kunstst.*, vol. 57, pp. 579–586, 2004.

[6] E. Dryzek, M. Wróbel, and E. Juszyńska-Gałazka, *Acta Phys. Pol. A*, vol. 132, pp. 1501–1505, 2017.

[7] A. Uedono, K. Sako, W. Ueno, and M. Kimura, *Compos. Part A: Appl. Sci. Manuf.*, vol. 122, pp. 54–58, 2019.

18. Time-Based Separation of Scattering and Capture Processes in NAA Based on Monte Carlo Simulations in Geant4 toolkit

Kamil Dulski¹, Wiktor Zantowicz¹

¹Faculty of Physics, Astronomy and Applied computer Science, Jagiellonian University, Poland

Neutron activation analysis (NAA) is a widely used method for the identification and quantification of elements, based primarily on two processes: neutron scattering and neutron capture. Each element is characterized by a unique spectrum; however, the analysis becomes challenging when spectral peaks overlap. Such a case is hydrogen and sulfur 2.23 MeV line superposition which is significant for the identification of illicit substances in aqueous environments.

We present an approach that separates spectrum originating from different processes using their temporal characteristics. Using Monte Carlo simulations, we will demonstrate how, by taking advantage of the time difference between neutron generation and the detection of a photon from neutron-matter interactions, we can successfully distinguish signals from neutron capture and inelastic neutron scattering. In addition to correctly quantifying the signals from individual atoms, this will also help reduce background from peak ambiguity, such as that for the 2.23 MeV peak mentioned above.



19. Developing analysis criteria for studies of CP symmetry with photons from o-Ps decay and Compton scattering with the Modular J-PET Detector

Kavya V. Eliyan , Magdalena Skurzok, Paweł Moskal On behalf of the J-PET Collaboration

¹*Faculty of Physics, Astronomy and Applied Computer Science, Jagiellonian University, Cracow, Poland.*

²*Center for Theranostics, Jagiellonian University, Cracow, Poland.*

Charge conjugation (C) and parity (P) transformation, both discrete symmetries, are coupled to generate Charge-Parity (CP) symmetry [1-8]. Charge conjugation (C) exchanges particles with their antiparticles, whereas parity (P) reflection reverses spatial coordinates [1-8]. Positronium is a suitable leptonic bound system to test CP discrete symmetry involving the correlations of photons momenta originating from ortho-Positronium (o-Ps) annihilation [1-8]. This work aims on developing new analysis criteria towards improving the sensitivity level for CP discrete symmetry studies in o-Ps decay. After the analysis selection chain, expectation value of CP odd operator ($\epsilon_i \cdot k_j$) will be calculated for each event, with three hits from o-Ps $\rightarrow 3\gamma$ decay and a fourth hit assigned as scattering to one of the annihilation photons. The goal is to achieve substantial (factor of 2 or more) improvement compared to previously published expectation value result of 0.0005 ± 0.0007 for the operator ($\epsilon_i \cdot k_j$) [7]. These studies will be carried out using the modular J-PET tomograph that has 20 times higher sensitivity for o-Ps registration [7, 9]. The modular J-PET tomograph is a newly developed, flexible, and portable variant of the J-PET detection system [9].

The authors acknowledge support from the National Science Centre (NCN), Poland through grants Nos.2019/35/B/ST2/03562 and 2021/42/ A/ST2/00423, the SciMat and qLife Priority Research Area budget under the auspices of the program Excellence Initiative — Research University at the Jagiellonian University.

- [1] P. Moskal et al., Acta Phys. Pol. B, vol. 47, p. 509, 2016.
- [2] W. Bernreuther, U. Löw, J. P. Ma, and O. Nachtmann, Z. Phys. C Part. Fields, vol. 41, p. 143, 1988.
- [3] B. K. Arbic et al., Phys. Rev. A, vol. 37, p. 3189, 1988.
- [4] S. D. Bass, S. Mariazzi, P. Moskal, and E. Stępień, Rev. Mod. Phys., vol. 95, p. 021002, 2023.
- [5] T. Yamazaki, T. Namba, S. Asai, and T. Kobayashi, Phys. Rev. Lett., vol. 104, p. 083401, 2010.
- [6] P. Moskal et al., Eur. Phys. J. C, vol. 78, p. 970, 2018.
- [7] P. Moskal et al., Nat. Commun., vol. 15, p. 78, 2024.
- [8] P. Moskal et al., Nat. Commun., vol. 12, p. 5658, 2021.
- [9] F. Tayefi Ardebili and P. Moskal, Bio-Algorithms Med-Syst., vol. 20, p. 9, 2024.

20. Miniature Scintillating Detectors and SiPMs: a brief Summary and a few Applications

Paolo Finocchiaro¹

¹INFN Laboratori Nazionali del Sud, Catania, Italy

During the last decades the development of silicon photo multipliers (SiPM) has reached a high degree of maturity. A wide variety of devices from several manufacturers is available nowadays on the market, both as single sensors and as arrays. Due to the low cost of the single sensor, along with its relevant performance and the limited requirement for supporting electronics, the development of high performance miniature radiation detectors has become possible and convenient. In this contribution the main characteristics of the SiPM will be described, and the implications of its coupling with miniature scintillators will be discussed highlighting benefits and drawbacks. A few application examples in different fields will be presented and current results will be shown, also with interesting perspectives in terms of Internet Of Things (IOT).



21. Direct imaging of the three-photon annihilation process beyond PET

Macoto Fujimoto, Riku Sato, Moh Hamdan, Kenji Shimazoe¹, Mizuki Uenomachi², Laura Stephenson, Archie Montgomery, Julien Bordes, Daniel Peter Watts

¹*The University of Tokyo, Japan*

²*Institute of Science Tokyo, Japan*

This research presents a novel imaging approach designed to visualize the three-photon annihilation of ortho-positronium (o-Ps), with the goal of obtaining diagnostic insights beyond conventional positron emission tomography (PET). Ortho-positronium, a metastable bound state of an electron and a positron, decays into three gamma photons, whose characteristics are influenced by environmental factors like oxygen concentration and molecular void size. To leverage this sensitivity, we introduce a direct imaging method that determines the location of each three-photon event based on energy and momentum conservation, without requiring traditional tomographic reconstruction or time-of-flight information.

A quadratic equation derived from the energy and momentum conservation of the detected photons forms the basis of a straightforward analytical model for estimating decay positions. The imaging system employs HR-GAGG scintillator arrays coupled with silicon-based multipixel photon counters (MPPCs) arranged in a PET-like ring configuration. Experimental validation was performed using ¹⁸F-FDG sources placed in 3D-printed phantoms with varying geometries. Three-photon images were generated and compared with simulation results to evaluate spatial resolution.

Furthermore, both porous and non-porous materials were imaged simultaneously to assess differences in the 3/2 annihilation ratio, which may serve as an indicator of tissue structure or hypoxic conditions. The system achieved spatial resolutions of approximately 2 mm axially and 8–11 mm transversely. The observed variation in decay ratios between materials agrees well with predictions and previous findings from positron annihilation lifetime spectroscopy (PALS).

These results confirm the feasibility of direct three-photon imaging using standard PET isotopes like ¹⁸F, and highlight its potential of providing complementary information on tissue hypoxia, morphology, and density.



22. Decay Law of Selected Fluorescent Substances

Francesco Giacosa¹, Milena Piotrowska¹, Krzysztof Kyzioł¹, Arthur Vereijken¹, Anna Kołbus¹, Karol Szary¹, Magdalena Płodowska¹

¹*Jan Kochanowski University, Kielce, Poland*

We present results from measurements of selected chemical compounds that decay via fluorescence photon emission. We examine to what extent the measured decay rates can be described by single- or double-exponential functions. We also investigate the emergence of non-exponential decay law that includes a power-law tail at long times.



23. Characterization of new SiC detectors for further experiments with exotic nuclei at barrier energies

J.F. González-Linares¹, T. Kurtukian-Nieto¹, L. Acosta¹, O. Tengblad¹, M. J. G. Borge¹, A. Nerio¹, and G. Pellegrini²

¹*Instituto de Estructura de la Materia, Consejo Superior de Investigaciones Científicas, Madrid, Spain*

²*Instituto de Microelectrónica de Barcelona-Centro Nacional de Microelectrónica, Consejo Superior de Investigaciones Científicas, Bellaterra, Barcelona, Spain*

In recent years, silicon carbide detectors (SiC) have become an alternative to conventional silicon detectors due to their similarity to diamonds but a lower cost [1]. Their radiation resistance and wide bandgap make SiC's semiconductor detectors with great possibilities like high intensity beam particle detection [2] or dosimetry for hadron therapy and FLASH radiotherapy [3]. The 4-H SiC prototypes developed at IMB-CNM [4-5] are being characterized in IEM-CSIC to study their viability to be part of the ISRS spectrometer [6], on its focal plane detection array and its beam profile monitors. This work is focused on the study of the energetic (about 40 keV of FWHM measured) and temporal resolution (lower than 200 ps reported [7]) of the devices, as well as the possibility of developing a SiC matrix system that allows spatial resolution in ion separation.

[1] M. De Napoli, "Frontiers in Physics," vol. 10, 2022.

[2] M. Christanell et al., "Journal of Instrumentation," vol. 17, no. 01, p. 1, 2022.

[3] C. Fleta et al., "Physics in Medicine and Biology," vol. 69, no. 9, 2024.

[4] I. Lopez Paz et al., "Scientific Reports," vol. 14, no. 1, 2024.

[5] I. Lopez Paz et al., "Journal of Instrumentation," vol. 19, no. 12, 2024.

[6] I. Martel et al., "Nuclear Instruments and Methods in Physics Research Section B," vol. 541, 2023.

[7] X. Zhang et al., "IEEE Transactions on Nuclear Science," vol. 60, no. 3, 2013.



24. Perspectives on Preclinical Molecular Imaging Research at the Radiopharmacy Centre, Medical University of Bialystok

Anna Gromotowicz-Poplawska^{1,2}, Izabela Suwda Kalita¹, Magdalena Bruzgo-Grzybko², Adam Olichwier¹

¹Radiopharmacy Centre, Medical University of Bialystok, Poland

²Department of Biopharmacy and Radiopharmacy, Medical University of Bialystok, Poland

The Radiopharmacy Centre at the Medical University of Bialystok, inaugurated in January 2024, is a newly established scientific unit designed to support the development and evaluation of novel radiopharmaceuticals through advanced preclinical research. Equipped with state-of-the-art infrastructure, the Centre houses fully operational laboratories for the synthesis, quality control, and preclinical assessment of radiopharmaceuticals, including facilities for in vitro and in vivo molecular imaging. The unit operates under national authorizations for radioactive isotope handling, genetic engineering (GMO/GMM), and experimental procedures involving laboratory animals (mice and rats), and is prepared for GMP-compliant manufacturing.

Key imaging capabilities include high-resolution PET/MR (3T) and SPECT/CT hybrid systems dedicated to small animal studies. These modalities enable detailed anatomical and functional imaging to support biodistribution studies, tumor visualization, pharmacokinetic modeling, and evaluation of new diagnostic markers. Current in vitro research focuses on identifying specific PET radiotracers targeting pancreatic and prostate cancer, using cell lines and radiometric techniques to assess receptor expression and ligand binding. The Centre is equipped with advanced devices including radiodetectors, flow cytometry, ELISA readers, and confocal microscopy systems.

The Centre integrates radiopharmacy expertise with advanced imaging and molecular biology tools, creating a unique platform for translational research in nuclear medicine – from bench to bedside. Its multidisciplinary team, comprehensive technical facilities and compliance with regulatory standards position it as a strategic national and international partner for academic and industrial collaborations in the development and validation of innovative diagnostic and therapeutic radiopharmaceuticals.

25. Impact of the Midkine expression on the uptake of [¹⁸F]FDG and [¹⁸F]FET in chicken chorioallantoic membrane glioblastoma models

Daniel Gündel ¹, Katarína Benčurová ^{2,3}, Silvester Bartsch ⁴, Joachim Friske ⁴, Maximilian Scheer ⁵, Sandra Leisz ⁵, Leonie Roß ⁵, Thomas H. Helbich ⁴, Markus Mitterhauser ^{2,3}, Marcus Hacker ², Klaus Kopka ^{1,6}, Andreas Maurer ^{1,7}, Cécile Philippe ^{2,3}, Theresa Balber ^{2,3}

¹*Helmholtz-Zentrum Dresden-Rossendorf (HZDR), Institute of Radiopharmaceutical Cancer Research, Department of Experimental Neurooncological Radiopharmacy, Leipzig/ Dresden, Germany*

²*Division of Nuclear Medicine, Department of Biomedical Imaging and Image-Guided Therapy, Medical University of Vienna, Vienna, Austria*

³*Joint Applied Medicinal Radiochemistry Facility, University of Vienna, Medical University of Vienna, Vienna, Austria*

⁴*Division of Molecular and Structural Preclinical Imaging, Department of Biomedical Imaging and Image-Guided Therapy, Medical University of Vienna, Vienna, Austria*

⁵*Department of Neurosurgery, University Medicine Halle, Halle, Germany*

⁶*Faculty of Chemistry and Food Chemistry, School of Science, TU Dresden, Dresden, Germany*

⁷*Leipzig University, Institute for Drug Discovery, Leipzig, Germany*

The utilization of fertilized chicken eggs, in which vascularized solid tumors can be grown on the chorioallantoic membrane (CAM), has recently garnered interest for the investigation of radiotracers [1, 2, 3]. In this study, we investigated the glucose and amino acid utilisation of chicken CAM glioblastoma (GBM) models and the influence of a human Midkine (hMDK) overexpression, a heparin-binding growth factor acting as a mediator for the acquisition of critical hallmarks of cancer, including cell growth, survival, metastasis, migration, and angiogenesis [4].

Eight different GBM cell lines were investigated regarding the MDK protein expression and secretion kinetics by Westernblot analysis. The human GBM cell lines U87 wildtype (U87(WT)), U87 overexpressing the human Midkine protein (U87(hMDK)), and the endogenic high midkine-expressing T98G were implanted on the CAM on embryo development day (EDD) 9 in a Matrigel® matrix. The injection of [¹⁸F]FDG or [¹⁸F]FET was performed between EDD15 to EDD18 followed by a simultaneous PET/MRI acquisition with a dedicated PET insert and an 86 mm PET-compatible coil (Bruker Biospin, Ettlingen, Germany) (n ≥ 4). For the semi-quantitative analysis of the radiotracer uptake with PMOD (v.4.205), a time frame of 30 to 40 min p.i. was reconstructed with a 3D MLEM algorithm.

The MDK expression and secretion kinetics are independent and vary between investigated cell lines. The uptake of [¹⁸F]FDG was comparable between U87(WT) and

U87(hMDK) tumors with 10.9 ± 2.9 and 9.4 ± 2.4 %ID/cm³ (p-value = 0.3232), respectively, whereas the uptake into MDK-expressing T98G tumors with 2.9 ± 0.8 %ID/cm³ was significantly lower (p-value < 0.001). In contrast to T98G, the tumor-to-blood and tumor-to-brain ratios indicated a high glucose utilisation of both U87 subclones. The [¹⁸F]FET uptake was also comparable between U87(WT) and U87(hMDK), with 4.7 ± 1.3 and 5.3 ± 1.1 %ID/cm³ (p-value = 0.4513), respectively, and again with 3.0 ± 1.1 %ID/cm³ significantly lower in T98G (p-values < 0.0300). Interestingly, a 3.8-fold higher [¹⁸F]FDG uptake compared to [¹⁸F]FET uptake in both U87 subclones (p-value = 0.0003) was determined, whereas the uptake of both radiotracers was comparable in T98G (p-value = 0.8846). The lower amino acid utilisation was reflected by the tumor-to-blood ratio of [¹⁸F]FET < 1 and the low brain uptake of [¹⁸F]FET favored a better tumor-to-brain ratio compared to [¹⁸F]FDG for all three tumor models.

The glucose and amino acid utilisation are independent of the hMDK overexpression, however, significant differences between glioma cell lines U87 and T98G could be demonstrated. The here investigated chicken CAM brain tumor models will be further used in the next steps for the development and evaluation of a novel class of hMDK-targeting radiotracers, which can provide further insights into the molecular development of brain tumors by means of non-invasive molecular imaging beyond glucose utilisation and amino acid uptake characteristics.

- [1] L. M. Smith et al., npj Imaging, vol. 1, no. 1, 2023.
- [2] K. Benčurová et al., Cancers, vol. 14, p. 5549, 2022.
- [3] G. Warnock et al., J. Nucl. Med., vol. 10, pp. 1782–1788, 2013.
- [4] P. S. Filippou et al., Oncogene, vol. 10, pp. 2040–2054, 2020.



26. Automated Simulation Workflow for 3D-Printed Scintillator Phantoms in Radiotherapy Planning

Jakub Hajduga¹, Bartłomiej Rachwał¹, Tomasz Szumlak¹, Tomasz Fiutowski¹, Kamila Kalecińska¹, Damian Kabat², Stefan Koperny¹, Maciej Kopeć¹, Dagmara Kulig¹, Bartłomiej Lach¹, Piotr Wiacek¹, Jakub Moroń¹, Bartosz Mindur¹

¹*AGH University of Science and Technology, Cracow, Poland*

²*Maria Skłodowska-Curie National Research Institute of Oncology Krakow, Poland*

Reconfigurable detector for the measurement of spatial radiation dose distribution for applications in the preparation of individual patient treatment plans was a research and development project aimed at improving radiation dose distribution measurement techniques for therapeutic applications. The core objective was to modernize current methodologies employed in individualized radiotherapy treatment planning by enabling precise, spatially-resolved, real-time dose measurements.

To this end, a prototype of a fully three-dimensional phantom composed of modular, 3Dprinted plastic scintillators was designed and constructed. This detector system allows for dose mapping at high spatial granularity. Complementing the hardware, a full simulation and data processing ecosystem was developed, with Monte Carlo simulations playing a central role in the calibration, optimization, and validation of the system. These simulations were implemented within a custom simulation platform named **G4RT**, built on top of the Geant4 toolkit. The simulation environment was tailored to the geometry and materials of the prototype phantom, including realistic representations of clinical treatment setups, such as beam-table interactions and attenuation profiles in tissue-equivalent media.

From a software architecture perspective, the project proposed a modular and reconfigurable approach to Geant4 simulation design. Unlike many existing systems constrained to standard geometries, the G4RT platform enables dynamic construction of complex, patient-specific detector arrangements. The geometry definitions, material databases, and simulation parameters are all externally configurable, allowing rapid iteration and scenario modeling. Integration with logging (LogSvc), configuration (TOML), and versioning mechanisms was a crucial part of maintaining transparency and reproducibility.

Another key development was the implementation of an automated geometry construction system designed to interface with CAD modeling software. Initially introduced during the **IMPRESS-U NAVA** project, this system enabled seamless integration of geometries created in **FreeCAD**. The approach relied on a structured, database-driven pipeline in which geometry metadata, positioning, and material assignments were extracted and processed from exported CAD data. This modular pipeline supported the automated construction of Geant4-compatible geometries

directly from CAD designs, minimizing manual intervention and ensuring reproducibility.

The framework was later extended and refined in the **Dose3D-Future** project to support models exported from **Autodesk Fusion 360**. The current implementation uses a **3MFbased CSV database** format as the intermediate representation. This format combines the geometric structure exported from Fusion (via the 3MF format) with associated metadata—such as volume names, material assignments, and hierarchical relationships—stored in structured CSV files. Material properties are automatically assigned using predefined mapping tables or explicit annotations, and spatial transformations are reconstructed from relative positioning information.

This automation drastically accelerates the preparation of patient-specific or experimentspecific simulations and ensures consistency between the physical phantom design and its digital counterpart. By embedding the geometry builder into the larger G4RT simulation ecosystem, the project established a scalable and reconfigurable architecture where CAD-driven geometry definitions are tightly coupled with physical modeling, logging, and configuration workflows.

An important component of the project also involved adaptation of the G4IAEphspReader to enable efficient simulation of particle phase-space (phsp) files. The reader was extended to allow dynamic filtering, precise scoring, and threading optimizations. This enabled realistic modeling of test beam conditions using experimentally obtained phsp data and enhanced the performance of simulations involving large datasets.



27. Study of Total-Body J-PET sensitivity as a function of the Ring Number

Sharareh Jalali¹, Martin Rädler¹, Keyvan Tayefi Ardebili^{1,2}, Pawel Moskal^{1,2}

¹*Faculty of Physics, Astronomy and Applied computer Science, Jagiellonian University, Cracow, Poland*

²*Center for Theranostics, Jagiellonian University, Cracow, Poland.*

Positron Emission Tomography (PET) is a key molecular imaging technique in nuclear medicine, enabling the detection of physiological changes in lesions prior to morphological alterations through the use of radiotracers. The Total-Body PET scanner, due to its extended detection area, offers significantly higher sensitivity, which is a key factor in overall tomographic performance [1]. The J-PET collaboration is currently developing a novel Total-Body PET prototype with an Axial Field Of View (AFOV) exceeding 250 cm, enabling low-dose imaging, reduced scan times, and dynamic imaging capabilities. A distinguishing feature of this design is the use of cost-effective plastic scintillators, which have the potential to make large-FOV PET scanners more widely accessible [1, 2]. One of the key performance metrics in PET is sensitivity, defined as the rate of true coincidence events detected per second per unit source strength [2, 3]. This study employs GATE simulations [4] to evaluate and compare the sensitivity of the Total Body J-PET and plastic-based brain PET scanner. Additionally, it investigates the combined sensitivity of brain PET integrated with the Total-Body J-PET system. The results of this study will be presented at the conference.

[1]. P. Moskal, E. Stępień, “Prospects and Clinical Perspectives of Total-Body PET Imaging Using Plastic Scintillators”, PET Clinics, 15 (2020) 439-452.

[2] P. Moskal et al., “Simulating NEMA characteristics of the modular total-body J-PET scanner—an economic total-body PET from plastic scintillators”, Phys. Med. Biol, 66 (2021) 175015.

[3]. J. Baran et al., “Realistic total-body J-PET geometry optimization: Monte Carlo study”, Medical Physics, 52 (2025) 2961-2975

[4]. David Sarrut et al., “The OpenGATE ecosystem for Monte Carlo simulation in medical physics”, Phys. Med. Biol, 67 (2022) 184001.



28. First Laboratory Tests of the SABAT Project Sensor with a D-T Neutron Generator

Mateusz Kaczmarek¹

¹Faculty of Physics, Astronomy and Applied computer Science, Jagiellonian University, Poland

Neutron Activation Analysis (NAA) is a non-destructive method enabling the determination of the elemental composition of substances and materials. This capability makes it suitable for identifying the contents of barrels sunk in the Baltic Sea that may contain hazardous substances. For this purpose, portable detectors of minimal size and without the need for cooling are required. In this study, a $\text{LaBr}_3\text{:Ce:Sr}$ scintillation detector with dimensions 3×3 inch was characterized, with optimal operating conditions and internal absorption determined. The obtained results were compared with earlier studies of a detector made of the same material with dimensions 2×2 inch. Furthermore, NAA was performed with a D-T neutron source (IGN-14) at IFJ PAN, using boric acid, seabed samples contaminated with fuel oil, and melamine as a nitrogen carrier. The measurements confirmed the feasibility and effectiveness of applying this detector in such analyses.



29. Plan-Guided Super-Resolution of Dose Distribution

Kamila Kalecińska¹, Bartosz Mindur¹; Bartłomiej Rachwa¹, Bartłomiej Lach¹,
Dagmara Kulig¹, Damian Kabat², Jakub Hajduga¹, Jakub Moroń¹, Maciej Kopeć¹,
Piotr Wiacek¹, Stefan Koperny¹, Tomasz Fiutowski¹, Tomasz Szumlak¹

¹AGH University of Science and Technology, Cracow, Poland.

²Maria Skłodowska-Curie National Research Institute of Oncology, Cracow,
Poland

This study centers on the design and evaluation of a Plan-Guided Super-Resolution framework, which seeks to enhance the fidelity and granularity of radiotherapeutic dose distribution measurements. These measurements are obtained from the Dose-3D-F detector, which is currently being developed as part of the project “*A reconfigurable detector for measuring the spatial distribution of radiation dose for applications in the preparation of individual patient treatment plans*” (<https://dose3d.fis.agh.edu.pl/>). The native resolution of the measurement is determined by the shape and size of a single detector cell (10 mm^3). By employing 3D convolutional neural networks, it is possible to increase this resolution to 1 mm^3 , ultimately contributing to improved accuracy in treatment planning. Comprehensive series of Monte Carlo simulations are conducted to produce training datasets as well as to validate the entire approach.



30. Design and construction of Cross-Staged Gantry System of Total-Body J-PET/CT Scanner for Motion Artifact Free anatomic and metabolic imaging

T. Kaplanoglu^{1,2}, P. Moskal^{1,2} on the behalf of the J-PET Collaboration

¹*Faculty of Physics, Astronomy and Applied Computer Science, Jagiellonian University, Cracow, Poland*

²*Center for Theranostics, Jagiellonian University, Cracow, Poland*

Total-body scanning rapidly acquires comprehensive, wide-volume metabolic data along with anatomical images using a lower radiopharmaceutical dosage [1,2], compared to conventional whole-body examinations performed through partial imaging steps. The Jagiellonian total-body PET/CT scanner [3,4] features a unique operational geometry that enables the examination of patients up to 2.5 meters in length without the need for discrete imaging approximations. To minimize artifacts caused by involuntary patient movement, both the patient and the examination table remain stationary during the scan, while the PET and CT gantries sequentially move around the patient from different axes. Due to the weight of the scanners and the precision required for the scanning processes, a custom-built mechanical motion system was developed. A custom motion system [5] was designed and constructed to move the total-body J-PET and CT devices along imaging X and Y axes within the examination room at the Center of Theranostics. The system consists of discrete rails and custom machine elements that allow the total-body J-PET and CT scanners to operate on the same platform. The designed system has been installed at the Theranostics Center in Kraków and will be used to integrate a commercial CT scanner with the total-body J-PET scanner, which was developed for research in both physics [6,7] and medicine [8,9] applications.

[1] A. Alavi, T. J. Werner, E. Ł. Stępień, and P. Moskal, *Bio-Algorithms Med-Syst.*, vol. 17, pp. 203–220, 2021.

[2] S. Vandenberghe, P. Moskal, and J. S. Karp, *EJNMMI Phys.*, vol. 7, p. 35, 2020.

[3] P. Moskal et al., *Phys. Med. Biol.*, vol. 66, no. 17, p. 175015, 2021.

[4] P. Moskal and E. Ł. Stępień, *PET Clin.*, vol. 15, no. 4, pp. 439–452, 2020.

[5] T. Kaplanoglu and P. Moskal, *Bio-Algorithms Med-Syst.*, vol. 19, no. 1, pp. 109–113, 2023.

[6] P. Moskal et al., *Nat. Commun.*, vol. 12, p. 5658, 2021.

[7] P. Moskal et al., *Nat. Commun.*, vol. 15, p. 78, 2024.

[8] P. Moskal et al., *Sci. Adv.*, vol. 7, p. eabh4394, 2021.

[9] P. Moskal et al., *Sci. Adv.*, vol. 10, p. eadp2840, 2024.



31. Optical properties and time-of-flight resolution of plastic scintillators for the total-body J-PET scanner

Łukasz Kapton^{1,2}, on behalf of the J-PET Collaboration

¹*Faculty of Physics, Astronomy and Applied Computer Science of the Jagiellonian University, Cracow, Poland*

²*Center for Theranostics, Jagiellonian University, Cracow, Poland*

Total-body Jagiellonian positron emission tomography (TB-J-PET) is based on long plastic scintillator strips [1]. The application of plastic scintillators as gamma detection material can decrease cost of the scanner [2] and increase its field-of-view. The J-PET scanner is capable of positronium imaging [3], measurements of entanglement of photons from positron-electron annihilation [4] and beam therapy monitoring [5]. The construction of long modules of the TB-J-PET requires use of plastic scintillators with high transparency to the emitted light [6] and with fast timing resolution. The two best manufacturers producing plastic scintillators with the highest transparency for the emitted light were selected for further research [7].

The aim of the research is to select the best plastic scintillator to be used in the construction of the TB-J-PET tomograph. The optical properties and timing resolution of six types of plastic scintillators manufactured by Eljen Technology, with dimensions of 6 mm × 30 mm × 500 mm, were measured. The emission spectra, transmittance at the wavelength of maximum emission through 6 mm thick scintillator, and technical attenuation length along 500 mm long scintillator, were measured on a linear CCD array spectrometer. The timing resolution was measured at three points along the scintillator using a setup consisting of silicon photomultipliers, oscilloscope, black box and collimated Na-22 source. The EJ-200 plastic scintillator has the best timing and optical properties for the TB-J-PET modules assembly.

We acknowledge support from the National Science Centre of Poland through grant No. 2023/07/X/ST11/01694.

[1] P. Moskal and E. Stępień, PET Clin., vol. 15, pp. 439, 2020.

[2] M. Dadgar et al., EJNMMI Phys., vol. 10, p. 62, 2023.

[3] P. Moskal et al., Sci. Adv., vol. 10, p. eadp2840, 2024.

[4] P. Moskal et al., Sci. Adv., vol. 11, p. eads3046, 2025.

[5] K. Parodi, T. Yamaya, and P. Moskal, J. Med. Phys., vol. 33, p. 22, 2023.

[6] Ł. Kapton, IEEE Trans. Nucl. Sci., vol. 67, no. 10, p. 2286, 2020.

[7] Ł. Kapton et al., Nucl. Instrum. Methods Phys. Res. A, vol. 1051, p. 168186, 2023.

32. Can decay gammas from radioactive ion beams enhance prompt gamma imaging?

Monika Kercz¹, Gabriel Ostrzolek¹, Daria Boscolo², Marco Durante², Ronja Hetzel², Rafał Lalik¹, Katarzyna Rusiecka¹, Aleksandra Wrońska¹

¹*Faculty of Physics, Astronomy and Applied Computer Science of the Jagiellonian University, Cracow, Poland*

²*GSI Helmholtz Centre for Heavy Ion Research, Darmstadt, Germany*

In recent decades, ion beam radiotherapy has gained popularity, i.e. both the number of patients treated annually and the number of clinical facilities in operation have increased. One of the key objectives to increase the precision of proton therapy is the development of a technique for online beam range verification. As the proton beam deposits its energy in the tissue, it can excite atomic nuclei, which then emit almost immediate (prompt) characteristic gamma radiation upon returning to the ground state. Additionally, if radioactive ions are used, they not only initiate nuclear excitations, but also decay, emitting additional gammas. These radiation channels carry information about the deposited dose distribution.

The SiFi-CC project aims to register such radiation to reconstruct the distribution of promptgamma vertices in real time, providing insight into the beam range. The detector is made of LYSO scintillating crystals and was developed specifically for prompt-gamma radiation detection. However, in the most recent experiment, we registered prompt and decay gammas from a phantom irradiated with a radioactive ¹¹C beam, using a coded mask setup.

Carbon ions offer greater precision in energy deposition compared to protons, which results in higher dose conformity, as well as better biological effectiveness. Using radioactive ions, the local dose in the tumour region where those ions stop, is enhanced due to their decay radiation. Moreover, such beams provide not only prompt gammas, but also annihilation gammas stemming from β^+ decay of ¹¹C, increasing the total gamma yield available for imaging. A series of measurements with a ¹¹C radioactive ion beam (RIB) was performed at GSI/FAIR, within the BARB (Biomedical Applications of Radioactive ion Beams) project.

The poster will present the results of the SiFi-CC subproject, including both simulations and preliminary experimental results.

33. Simulated Signal Database for Improved Resolution in Position Sensitive Planar Germanium Detector

Priyanka Khandelwal¹, S. Mandal¹, R. Palit², J. Gerl³, A. Sharma⁴

¹*Department of Physics & Astrophysics, University of Delhi, New Delhi, India*

²*Department of Nuclear and Atomic Physics, Tata Institute of Fundamental Research, Mumbai, India*

³*GSI Helmholtzzentrum für Schwerionenforschung, Darmstadt, Germany*

⁴*Universite Paris-Saclay, CNRS/IN2P3, IJCLab, Orsay, France*

The progress in gamma-ray spectroscopy has been greatly influenced by the introduction of highly segmented germanium detectors. Their integration with advanced methods like pulse shape analysis (PSA) and gamma-ray tracking (GRT) has opened up new possibilities for high-resolution gamma-ray imaging. However, the accuracy of pulse shape analysis is fundamentally limited by the availability and quality of realistic signal database, which are often difficult to generate experimentally with sufficient resolution and coverage.

To address this, we have developed a detailed simulation to construct a comprehensive signal database for a double-sided, planar segmented HPGe detector with 10 orthogonal strips along both X and Y directions. The whole simulation framework has been developed with the help of two simulation tools. Gamma-ray interactions were simulated using the Geant4 toolkit, while charge transport modeling was carried out using the open-source Julia package SolidStateDetectors.jl [1]. Detector specific electric field and potential distributions were calculated on an adaptive grid, incorporating full geometry and biasing conditions provided by the manufacturer. Charge carrier dynamics including drift and diffusion were simulated using mobility parameters from the AGATA Detector Library (ADL) [2]. The resulting signals induced at AC and DC electrodes were convoluted with a preamplifier response for including electronics effects [3]. The relationship between pulse shapes has been analyzed in more detail by examining the variation in rise-time between signals induced on opposing detector surfaces, as a function of depth, for different strips. This generated database enables dense spatial sampling of interaction points and provide waveforms necessary for PSA. Validation is currently underway through comparison with scanning data from the planar segmented PSPGe detector at GSI, Germany [4]. By bridging the gap between simulation and experiment, our work provides a solution to support gamma-ray reconstruction in future tracking arrays. Full simulation and comparison results will be discussed in detail during the conference.

[1] I. Abt et al., J. Instrum., vol. 16, p. P08007, 2021.

[2] B. Bruyneel et al., Eur. Phys. J. A, vol. 52, p. 70, 2016.

[3] E. Rintoul et al., Nucl. Instrum. Methods Phys. Res. A, vol. 987, p. 164804, 2021.

[4] A. Sharma et al., Nucl. Instrum. Methods Phys. Res. A, vol. 1051, p. 168233, 2023.

34. Titanium-Scandium Radionuclide Generator: A New Approach for Sustainable Isotope Production

Aleksander Khreptak^{1,2}, Paweł Moskal, Ewa Stępień^{1,2}

¹Faculty of Physics, Astronomy and Applied Computer Science, Jagiellonian University, Cracow, Poland

²Center for Theranostics, Jagiellonian University, Cracow, Poland

Advancing positronium imaging requires a reliable supply of suitable radionuclides and efficient radiolabeling strategies. The poster will present the concept of a titanium-scandium radionuclide generator as a practical and sustainable solution for producing scandium-44, a radionuclide offering a unique prompt gamma emission for triple-photon detection. This generator system could provide a steady, on-demand source of high-purity ⁴⁴Sc for the synthesis of novel positronium imaging agents. This approach has the potential to simplify logistics, reduce production costs, and support the wider adoption of positronium imaging in both preclinical and clinical settings.



35. MERMAID – prototype PET scanner for small aquatic animals

Magdalena Kolodziej, Steven Seeger, Hong Phuc Vo, Rebecca Kantorek, Jorge Roser, Christian Schmidt, Magdalena Rafecas

Universität zu Lübeck, Germany

MERMAID (Multi-Emission Radioisotopes - Marine Animal Imaging Device) is the first PET scanner prototype dedicated to small aquatic animals. Particularly, MERMAID aims to support biomedical research using zebrafish as a model of human diseases, as well as marine biology research and sustainable aquaculture.

Even though there are small-animal PET scanners commercially available, they are optimised for rodents, so their spatial resolution might be insufficient for small fish. Other requirements related to imaging aquatic animals further restrict their use. Therefore, there is a need for a dedicated system. The current prototype, with four crystal modules composed of LYSO crystals and SiPMs, has proved its capability of imaging sub-mm structures; PET scans of radioactive phantoms and zebrafish have been successfully conducted. The current field-of-view is being extended with new crystal modules, currently in the assembly process.

In the talk, I will present the MERMAID system, including characterization and status of the latest development and show reconstructed images of fish-like phantoms and zebrafish.



36. Silicon as beam-activated tumour tracer for online proton therapy monitoring – experimental study

Magdalena Kolodziej^{1,2}, Aleksandra Wrońska²

¹*Universität zu Lübeck, Germany*

²*Faculty of Physics, Astronomy and Applied Computer Science, Jagiellonian University, Cracow, Poland*

In this study, the feasibility of utilizing silicon as a new kind of tumour tracer in proton therapy was experimentally investigated. Our approach can potentially become a method of online monitoring in proton therapy, allowing for more efficient healthy tissue sparing and thus for better and safer treatment. So far, there is no method of online proton beam monitoring applied routinely in clinics. This results in a necessity to apply safety margins, increasing the risk of long-term side effects. The underlying principle of the tracer method is that certain elements emit prompt gamma (PG) quanta of characteristic energy when irradiated with a proton beam. It is also necessary that the cross section for PG emission peaks for low energies, then the PG vertex distribution will follow the dose distribution with good approximation. Previous research indicated silicon as the optimal element for this purpose. Optimal tracer concentrations were also determined. If the tracer is selectively delivered to the tumour volume, one expects to see the silicon peak in the PG energy spectrum only when the Bragg peak reaches the tumour volume, thus providing feedback for the clinician in real time. An experiment in clinical conditions was conducted to quantify this effect (predicted by simulations): a PMMA phantom with a silicon-doped insert was irradiated with beams of different energies (with the Bragg peak either inside or outside the insert volume) and a high purity germanium detector was placed to the side of the phantom to register the PG spectrum. Additional measurements were done with an extra PMMA plate in front of the phantom, to induce a beam range shift. In my talk, I will present preliminary results from this experiment and discuss the feasibility of the method for use in proton therapy monitoring.



37. Fragmentation measurements for particle therapy with the FOOT experiment

Aafke Kraan

INFN - Sezione di Pisa, Italy

Fragmentation measurements FOOT (FragmentatiOn Of Target) is an innovative experiment in applied nuclear physics, dedicated to the understanding of nuclear fragmentation processes. The understanding of such processes is relevant in oncological treatments with hadron beams and in the field of radiation protection in space. The FOOT physics program foresees a set of measurements conducted in both direct and inverse kinematics, employing particle beams and targets similar to the composition of human tissues from one side and spacecraft shielding materials on the other.

The main goal of the experiment is to measure double differential cross-sections as a function of scattering angle and fragment energy within the 100-800 MeV/u range, achieving a precision level exceeding 5%. At present, the FOOT Collaboration has developed two experimental set-ups: one based on nuclear emulsions devoted to charges $Z \leq 4$ and another based on electronic detectors for fragments with $Z \geq 2$. In this presentation we will give an overview of the status of the experiment, present some preliminary and recent results, and give details on the upcoming experimental campaigns.



38. Usage of DL-based portal dose images for treatment error detection with transit dosimetry in radiotherapy

Aafke Kraan

INFN - Sezione di Pisa, Italy

Electronic portal imaging devices (EPIDs) can be employed for performing transit in-vivo dosimetry. However, a significant drawback of conventional amorphous silicon EPID detectors in this context is their non-linear response to water-equivalent dose. This necessitates complex calibration and correction processes, reducing their feasibility for routine clinical implementation. In this study, we propose a deep learning (DL) approach designed to reconstruct water-equivalent dose from transit EPID images, using both image data and dose simulations from a treatment planning system (TPS). The model was trained on a comprehensive dataset comprising more than 200 EPID acquisitions and corresponding portal dose outputs generated by the Monaco TPS, encompassing various phantom types and irradiation field configurations. A 2D U-Net architecture was developed to convert EPID transit images into water-equivalent portal dose maps. The model's performance was assessed using mean absolute error (MAE) and 2D gamma index analysis, applying 3mm/3% and 5mm/5% evaluation criteria. The average MAE across all test samples was 3.9×10^{-3} cGy. Gamma index passing rates averaged $94.5 \pm 2.0\%$ and $99.6 \pm 0.3\%$ for the 3mm/3% and 5mm/5% thresholds, respectively. Median gamma pass rates were 98.2% and 100% for the two criteria, underscoring the model's high accuracy in dose reconstruction from EPID images. Furthermore, the model generates portal dose predictions in less than one second, indicating its potential for real-time clinical application. Overall, our DL framework provides a fast and reliable method for estimating water-equivalent dose from EPID images, presenting a viable path toward more accurate and efficient in-vivo dosimetry.



39. Normalisation Strategies in ToF-SIMS Analysis of Liver Tissue - Critical Impact on Comparative Molecular Profiling in a Diabetic Rat Model

Michalina Kaźmierczak¹, Magdalena E. Skalska^{1,2}, Marcela Capcarova⁴, Anna Kalafova⁴, Peter Massanyi⁴, Klaudia Jaszcza⁵, Dorota Wojtysiak³

¹*Faculty of Physics, Astronomy and Applied Computer Science, Jagiellonian University, Cracow, Poland;*

²*Centre for Theranostics, Jagiellonian University, Cracow, Poland;*

³*Department of Genetics, Animal Breeding and Ethology, University of Agriculture in Cracow, Cracow, Poland*

⁴*Institute of Applied Biology, Faculty of Biotechnology and Food Sciences, Slovak University of Agriculture in Nitra, Nitra, Slovak Republic*

⁵*Department of Animal Physiology and Endocrinology, University of Agriculture in Cracow, Cracow, Poland*

Time-of-flight secondary ion mass spectrometry (ToF-SIMS) enables high-resolution molecular imaging of biological tissues, providing unique insights into chemical composition at the microscale. In this technique, the method of data normalisation plays a pivotal role in the reliability of biological comparisons, particularly in complex tissue analyses. In this study, we evaluated the influence of different normalisation approaches on the interpretation of ToF-SIMS results obtained from liver samples of diabetic rats treated with metformin or flaxseed mucilage.

Liver sections were analysed in both ion modes (positive, negative) using ToF-SIMS 5, and ROIs ($150 \times 150 \mu\text{m}^2$) were extracted from larger scanned areas to avoid topographic and edge artefacts. Several normalisation strategies were applied: total ion count (TIC), ion dose normalisation, and relative scaling to control groups. The impact of each method was assessed through quantitative comparison of ion group abundances (amino acids, lipids, metal ions, carbon-containing ions) and group separation capacity.

Our results indicate that TIC normalisation improves comparability across samples by reducing instrumental and matrix effects but may obscure biologically relevant changes. Normalisation to control group levels highlighted treatment-induced differences more clearly, particularly the elevated metal ion signals in metformin-treated livers and preserved amino acid profiles in flaxseed groups. Normalisation to ion dose provided consistent results in spatial analyses but was less sensitive in group discrimination.

This study underscores the critical importance of normalisation selection in ToF-SIMS-based tissue profiling. The appropriate strategy choice can enhance the biological relevance and reproducibility of findings, especially in comparative pharmacological studies involving subtle metabolic changes.

40. Ex-Vivo Positronium Lifetime Imaging with ^{44}Sc Using J-PET Scanner

Karol Kubat^{1,2}, Manish Das^{1,2}, Sushil Sharma^{1,2}, Ewa Ł. Stępień^{1,2} and Pawel Moskal^{1,2} On behalf of the J-PET Collaboration

¹*Faculty of Physics, Astronomy and Applied Computer Science, Jagiellonian University, Cracow, Poland*

²*Centre for Theranostics, Jagiellonian University, Cracow, Poland*

Positronium Lifetime Imaging (PLI), an advanced extension of Positronium Emission Tomography (PET), is an emerging diagnostic modality [1,2,3]. It has potential to probe nano-scale environmental properties such as hypoxia, tumour microenvironment pathology by mapping the spatial distribution of Ps lifetime in biological tissues [4, 5, 6].

Despite the common consensus on its advantages and ongoing progress in adaptation of reconstruction algorithms and detector technology, PLI faces slow translation in clinical applications mainly due to two reasons: (1) measurement of nano-second positronium lifetimes requires fast gamma-ray detectors, and (2) new radioisotopes that provide both medically suitable half-life and high positron yield accompanying a prompt gamma signal for Ps lifetime estimation. The first in-vivo results on PLI of human brain was reported by J-PET collaboration using ^{68}Ga radioisotope [7]. However, the low prompt gamma yield of ^{68}Ga , only a $\sim 1.34\%$ prompt- γ branching ratio, poses challenges for accurate lifetime estimation due to limited statistics [8].

To address this, ^{44}Sc has emerged as a highly promising isotope for PLI [9], boasting an optimal decay profile: a clinically suitable half-life of 4.04 hours, an ultrashort deexcitation delay of 2.61 ps, and a 100% decay probability producing a single, high-energy (1157 keV) prompt gamma following positron emission [8].

In this work, we report the successful application of PLI using ^{44}Sc , performed with the state-of-the-art Modular J-PET tomograph, featuring triggerless data acquisition enabling simultaneous multiphoton detection [7]. For this study ^{44}Sc was produced at the Heavy Ion Laboratory in Warsaw and transported to Jagiellonian University in Kraków. Four phantoms containing cardiac myxoma tissue, blood thrombi, adipose tissue, and Fused Silica were used, where the Fused Silica serving as the certified material with a known o-Ps lifetime for quality control. Event selection was based on the simultaneous detection of two 511 keV photons and one de-excitation photon, enabling the reconstruction of positronium lifetime images. The reconstructed annihilation positions, obtained using the two 511 keV photons along with the positron lifetime, was used to identify regions of interest (ROIs) in image samples. Whereas the o-Ps lifetime was estimated utilizing the registration time of an additional prompt gamma as the o-Ps formation time. The obtained o-Ps lifetime shows good agreement with previously reported values for biological tissues [3, 10].

In this presentation, we will show the first-ever demonstration of ex-vivo PLI with ^{44}Sc ,

marking a significant advancement and opening new possibilities for developing PLI for clinical applications.

This work was supported by the National Science Centre of Poland (Grants: 2021/42/A/ST2/00423, 2021/43/B/ST2/02150, 2022/47/I/NZ7/03112), SciMat and qLife under the Excellence Initiative at Jagiellonian University, and PLGrid (ACK Cyfronet AGH, PLG/2024/017688).

- [1] P. Moskal, Proc. IEEE Nucl. Sci. Symp. Med. Imaging Conf. (NSS MIC), Manchester, pp. 1–3, 2019
- [2] P. Moskal et al., IEEE Trans. Radiat. Plasma Med. Sci., early access, 2025
- [3] P. Moskal et al., Sci. Adv., vol. 7, p. eabh439, 2021.
- [4] P. Moskal et al., EJNMMI Phys., vol. 10, p. 22, 2023.
- [5] P. Moskal et al., Bio-Algorithms Med-Syst., vol. 17, no. 4, pp. 311–319, 2021.
- [6] P. Moskal et al., Nat. Commun., vol. 12, p. 5658, 2021.
- [7] P. Moskal et al., Sci. Adv., vol. 10, p. adp2840, 2024.
- [8] M. Das et al., Bio-Algorithms Med-Syst., vol. 19, pp. 87–95, 2023.
- [9] P. Moskal and E. Stępień, PET Clin., vol. 15, p. 439, 2020.
- [10] A. V. Avachat, K. H. Mahmoud, A. G. Leja, et al., Sci. Rep., vol. 14, p. 21155, 2024.



41. Measuring the degree of entanglement in matter using a plastic-scintillator based PET scanner

D. Kumar^{1,2}, S. Sharma^{1,2} and P. Moskal^{1,2}, on behalf of the J-PET collaboration

¹*Faculty of Physics, Astronomy, and Applied Computer Science, Jagiellonian University, Cracow, Poland.*

²*Center for Theranostics, Jagiellonian University, Cracow, Poland*

Understanding quantum entanglement of photons produced in positron–electron annihilation offers exciting prospects for both fundamental physics and quantum-enhanced medical imaging [1,2]. According to quantum electrodynamics, annihilation photons from the singlet state of positronium decay exhibit entangled polarization [3]. This entangled nature can be accessed by measuring the correlation between their polarization states. However, the high energy of these photons (511 keV) makes it impossible to use traditional polarizers. We address this issue by utilizing Compton scattering as a polarization analyser, exploiting the strong dependence of the scattered photon direction on the polarization of incident photon [4].

In this study, a plastic-scintillator-based PET scanner (J-PET) is used, which is particularly well-suited for this research, as photons predominantly register via Compton scattering, enabling the measurement of entanglement properties of 511 keV photons [5,6]. The recent results demonstrated the non-maximal entanglement between photons, when positrons annihilate in a porous polymer medium, with the observed degree of correlation sensitive to the annihilation environment [7]. These findings pave the way for further investigations into how entanglement varies across different physical and chemical surroundings. This is crucial because the degree of quantum correlation is expected to change with different annihilation modes within the material, potentially introducing new contrast mechanisms for quantuminformed imaging [7,8].

This presentation will highlight the advanced features of the J-PET detector and new findings on the polarization correlation of annihilation photons in medium and future goals [2,6,7].

We acknowledge support from the Foundation for Polish Science through the TEAM POIR.04.04.00-00-4204/17 program, the National Science Centre of Poland through Grants No. 2019/35/B/ST2/03562, 2021/42/A/ST2/00423, 2021/43/B/ST2/02150, 2023/50/E/ST2/00574, 2024/53/N/ST2/04279 and the SciMat and qLife Priority Research Area budget under the program Excellence Initiative—Research University at Jagiellonian University.

- [1] P. Moskal, Proc. 2018 IEEE Nucl. Sci. Symp. Med. Imaging Conf. (NSS MIC), pp. 1–4, 2018.
- [2] S. D. Bass et al., Rev. Mod. Phys., vol. 95, p. 021002, 2023.
- [3] H. S. Snyder, S. Pasternack, and J. Hornbostel, Phys. Rev., vol. 73, p. 440, 1948.
- [4] O. Klein and Y. Nishina, Z. Phys., vol. 52, p. 853, 1929.
- [5] S. Niedzwiecki et al., Acta Phys. Pol. B, vol. 48, p. 1567, 2017.
- [6] P. Moskal et al., Eur. Phys. J. C, vol. 78, p. 970, 2018.
- [7] P. Moskal et al., Sci. Adv., vol. 11, p. eads3046, 2025.
- [8] P. Moskal, Physics, vol. 17, p. 138, 2024.



42. Nanobrachytherapy of Triple-Negative Breast Cancer and Glioblastoma Multiforme Using Auger Emitters

Emilia Majka¹, Rafał Walczak¹, Penelope Bouziotis², Evangelia-Alexandra Salvanou², Aleksander Bilewicz¹, Agnieszka Majkowska-Pilip¹

¹*Institute of Nuclear Chemistry and Technology, Warsaw, Poland*

²*Radiochemical Studies Laboratory, Institute of Nuclear and Radiological Sciences & Technology, Energy & Safety (INRASTES) of the National Center for Scientific Research “Demokritos”, Athens, Greece*

Cancers that do not exhibit overexpression of specific receptors are a significant challenge for the development of novel radiopharmaceuticals. Metastatic triple-negative breast cancer (TNBC) is associated with a 12% survival rate [1], while glioblastoma multiforme (GBM) has a mortality rate of 93% [2].

Nanobrachytherapy enables the intratumoral administration of radiopharmaceuticals without the necessity of targeting specific receptors. Mercury radionuclides ^{197/197m}Hg demonstrate remarkable efficacy, generating 42.6 Auger electron emissions per decay. By leveraging Auger electron-emitting radionuclides with their high linear energy transfer (LET) that causes DNA double-strand breaks, we can improve nanobrachytherapy by combining ^{197/197m}Hg with gold nanoparticles (AuNPs).

The Au(^{197/197m}Hg)NPs-PEG radioconjugate was synthesized and subsequently evaluated in vitro for its therapeutic potential on MDA-MB-231 and T98G cancer cell lines. Cell cultures underwent internalization, subcellular fractionation, MTS assay, and spheroid studies. Additionally, flow cytometry analysis was used to evaluate the apoptosis and cell cycle of treated cells. Furthermore, the -H2AX phosphorylation technique was employed to measure the number of DNA double-strand breaks caused by the radioconjugate, revealing a significant level of DNA DSBs. Ex vivo biodistribution and therapeutic efficacy studies were conducted on mice bearing 4T1 tumors at the Radiochemical Studies Laboratory, INRASTES, NCSR Democritos in Athens, Greece.

Au(^{197/197m}Hg)NPs-PEG showed significant internalization in both cell lines. In MDA-MB-231, 87.51 ± 0.16% internalization occurred after 24 hours, with 26.6 ± 0.48% localized in the cell nucleus. It caused a highly effective DNA double-strand break, which was 63 times higher than that of the control group after 24 hours. In the biodistribution study on mice, we established that most Au(^{197/197m}Hg)NPs-PEG remained in the tumor two hours post-injection. The radioconjugate with a dose of 10 MBq indicated a 31.61 ± 6.83% reduction in tumor growth index (TGI) after 18 days of treatment.

We conjugated efficient Auger-electron emitting radionuclides $^{197/197\text{m}}\text{Hg}$ —onto gold nanoparticles (AuNPs) for the nanobrachytherapy of TNBC and GBM. The in vitro and in vivo potential of Au($^{197/197\text{m}}\text{Hg}$)NPs-PEG has shown significant promise. A therapeutic efficacy ex vivo study on mice using smaller doses of this radioconjugate is scheduled to be conducted.

Acknowledgments

This research was financed by the PRELUDIUM 20 grant 2021/41/N/ST5/00322 from the National Centre of Science, Poland.

[1] Triple-negative Breast Cancer. [Online]. Available: www.cancer.org/cancer/types/breast-cancer/about/types-of-breast-cancer/triple-negative.html [Accessed: Feb. 17, 2025].

[2] Grade 4 – Glioblastoma (GBM). [Online]. Available: www.braintumor.org [Accessed: Feb. 17, 2025].



43. High Precision X-ray Spectroscopy: from Kaonic Atoms to Societal Applications

Simone Manti

INFN- Laboratori Nazionali di Frascati, Italy

Understanding the strong interaction at low energies remains one of the fundamental challenges in nuclear and particle physics. Experimental studies of low-energy kaon-nucleon and kaon-nucleus interactions provide critical insights for advancing Quantum Chromodynamics (QCD), with far-reaching implications from the structure of nuclei to the physics of neutron stars. At the DANE collider in Frascati (Italy), the SIDDHARTA and SIDDHARTA-2 collaborations have leveraged state-of-the-art X-ray detection technologies, such as Silicon Drift Detectors, to achieve unprecedented precision in the spectroscopy of exotic atoms, most notably kaonic hydrogen, deuterium and neon. These efforts are enabling the world's first measurements of kaonic deuterium, a milestone for the field. In this contribution, I will present the physics motivation for studying kaonic atoms, describe the experimental setup and detector developments, and discuss recent results on kaonic neon and future directions. In addition, I will report on the development of a novel setup for high-resolution X-ray spectroscopy based on a mosaic crystal, designed to push the limits of energy resolution in exotic atom experiments. This integrated approach, combining innovative detection systems and advanced spectroscopic methods, opens new avenues for precision measurements in understanding the role of strangeness in the universe, with, in the same time, numerous possible societal applications.



44. Preliminary tests of positronium gathering in microcavities connected to nanochannels

Sebastiano Mariazzi¹, Roberto Sennen Brusa^{1,2}, Ahmad Chehaimi¹, Erika Socal¹

¹*University of Trento, Italy*

²*INFN-TIFPA, Italy*

Nanochanneled silicon samples produced via electrochemical etching have proven to efficiently convert positron to positronium in both reflection (positronium emitted from the same side of positron implantation [1-3]) and transmission geometry (positronium emitted from the opposite side of positron implantation [4]). In the last decade, these positron/positronium converters have been successfully employed for the production and emission into the vacuum of positronium for experiments of positronium laser excitation [5-8], antihydrogen production [9], and positronium laser cooling [10]. Further experiments of positronium inertial sensing [11] and entanglement of the 3 gammas generated by positronium self-annihilation [12] based on the use of such samples are planned.

Here, we investigate the potential of combining electrochemical etching and ultrafast laser direct writing [13] to fabricate silicon samples containing a network of nanochannels connected to buried microcavities. The aim is to gather positronium in these microcavities for future studies on positronium spectroscopy within the microcavities [14] and positronium-positronium interaction [15] with the new bunched positron beam at the Antimatter Laboratory of Trento [16, 17]. The structure of the produced samples was explored via Transmission Electron Microscopy and Scanning Electron Microscopy. Positronium formation and gathering in the microcavities were investigated via Positron Annihilation Spectroscopy. Samples, where over 20% of implanted positrons form positronium self-annihilating via 3 gammas inside microcavities, were obtained.

- [1] S. Mariazzi, P. Bettotti, S. Larcheri et al., Phys. Rev. B, vol. 81, p. 235418, 2010.
- [2] S. Mariazzi, P. Bettotti, R. S. Brusa et al., Phys. Rev. Lett., vol. 104, p. 243401, 2010.
- [3] S. Mariazzi, P. Bettotti, R. S. Brusa et al. (AEgIS Collaboration), J. Phys. B, vol. 54, p. 085004, 2021.
- [4] S. Mariazzi, B. Rienäcker, R. Magrin Maffei et al., Phys. Rev. B, vol. 105, p. 115422, 2022.
- [5] S. Aghion, R. Caravita, M. Doser et al. (AEgIS Collaboration), Phys. Rev. A, vol. 94, p. 012507, 2016.
- [6] S. Aghion, R. Caravita, M. Doser et al. (AEgIS Collaboration), Phys. Rev. A, vol. 98, p. 013402, 2018.
- [7] C. Amsler, M. Antonello, A. Belov et al. (AEgIS Collaboration), Phys. Rev. A, vol. 99, p. 033405, 2019.
- [8] M. Antonello, C. Amsler, A. Belov et al. (AEgIS Collaboration), Phys. Rev. A, vol. 100, p. 063414, 2019.
- [9] C. Amsler, M. Antonello, A. Belov et al. (AEgIS Collaboration), Commun. Phys., vol. 4, p. 19, 2021.
- [10] L. T. Glöggler, C. Amsler, M. Antonello et al. (AEgIS Collaboration), Phys. Rev. Lett., vol. 132, p. 083402, 2024.
- [11] S. Mariazzi, R. Caravita, M. Doser et al., Eur. Phys. J. D, vol. 74, p. 79, 2020.
- [12] S. D. Bass, S. Mariazzi, P. Moskal et al., Rev. Mod. Phys., vol. 95, p. 021002, 2023.
- [13] I. T. Sorokina, N. Tolstik, R. A. Richter et al., Proc. VII Int. Symp. Ultrafast Dynamics Metastability, Crete, Greece, pp. 84–85, Jun. 2022.
- [14] B. S. Cooper, J. P. Boilot, C. Corbel et al., Phys. Rev. B, vol. 97, p. 205302, 2018.
- [15] D. B. Cassidy, S. H. M. Deng, R. G. Greaves et al., Phys. Rev. Lett., vol. 95, p. 195006, 2005.

- [16] L. Povoło, S. Mariazzi, L. Penasa et al., Phys. Rev. Accel. Beams, vol. 26, p. 051601, 2023.
- [17] L. Povoło, S. Mariazzi, M. Bettonte et al., Nucl. Instrum. Methods B, vol. 552, p. 165376, 2024.



45. Development of a high-quality, energy-tunable positronium beam via photodetachment of positronium negative ions

Koji Michishio

National Institute of Advanced Industrial Science and Technology, Japan

When an electron binds to its antimatter counterpart, the positron, they form a hydrogen-like bound state known as positronium (Ps). Although Ps decays into gamma-rays via annihilation within a short lifetime, it behaves as an electrically neutral particle until annihilation. Ps atoms are formed in the final stages of radiation-induced processes involving positron injection into matter, making them an important subject of study in positron-related radiation science. Ps has been increasingly utilized as a probe in applied research, such as the evaluation of pore structures in polymers and porous materials [1]. In recent years, its potential use in acquiring biological information in positron emission tomography (PET) has also attracted growing interest [2,3]. To advance such applications, it is essential to accumulate fundamental data on interactions between Ps and atoms/molecules. An energy-tunable Ps beam is a powerful tool for studying these interactions over a wide range of collision energies. However, due to its short annihilation lifetime and neutral charge, the generation of Ps beams has posed significant technical challenges.

To overcome this challenge, we have demonstrated a method for producing Ps beams using positronium negative ions, which are bound states consisting of a Ps atom and an additional electron. Owing to their negative charge, Ps negative ions can be accelerated to a desired energy using an electric field. By subsequently removing the extra electron via laser photodetachment [4], we successfully generated a monoenergetic, energy-tunable Ps beam [5]. Furthermore, by enhancing the system performance through the implementation of a trap-based positron beam, we developed a high-quality, energy-tunable positronium beam suitable for applied research [6,7]. The resulting beam is expected to contribute not only to fundamental science but also to the development of novel analytical techniques for material characterization

[1] Y. C. Jean, *Microchem. J.*, vol. 42, p. 72, 1990.

[2] S. D. Bass, S. Mariuzzi, P. Moskal et al., *Rev. Mod. Phys.*, vol. 95, p. 021002, 2023.

[3] P. Moskal, E. Stępień, L. Chmielewski et al., *Sci. Adv.*, vol. 10, p. eadp2840, 2024.

[4] K. Michishio, T. Tachibana, A. Yagishita et al., *Phys. Rev. Lett.*, vol. 106, p. 153401, 2011.

[5] K. Michishio, H. Saito, T. Tachibana et al., *Appl. Phys. Lett.*, vol. 100, p. 254102, 2012.

[6] K. Michishio, T. Yamazaki, A. Miyazaki et al., *Rev. Sci. Instrum.*, vol. 90, p. 023305, 2019.

[7] K. Michishio, T. Yamazaki, T. Namba et al., *Phys. Rev. Lett.*, vol. 132, p. 203001, 2024.

46. In-beam PET monitoring during radioactive ion beams irradiation for real-time dose discrepancies and anatomical change detection

Martina Moglioni¹, Daria Boscolo¹, Olga Sokol¹, Katia Parodi⁴, Uli Weber¹, Marco Durante¹

¹GSI Helmholtz Centre for Heavy Ion Research, Darmstadt, Germany

²Ludwig-Maximilians-Universität München, LMU, Munich, Germany

In-beam Positron Emission Tomography (IB-PET) enables real-time monitoring of charged particle therapy by detecting 511 keV annihilation photons resulting from decays of radioisotopes produced during nuclear interactions of the primary beam with patient tissue. However, in proton and stable ^{12}C -ion beams treatment, IB-PET is limited by low count rates, biological washout, and broad activity distributions. Radioactive ion beams (RIBs), such as ^{11}C , while not yet used in clinical treatments, would yield an improved signal and a closer match with the dose fall-off, enabling a more precise in vivo beam range monitoring and tumor control. This study investigates whether RIBs can enable quasi-instantaneous detection of dose deviations and anatomical changes during treatment and compares the results with that of protons and ^{12}C beams.

We used the FLUKA Monte Carlo simulation tool to model isotope production and decays (referred here as the IB-PET signal) for 8 head-and-neck tumor treatments using proton, ^{12}C , and ^{11}C -ion beams. Simulations accounted for realistic clinical conditions, including anatomical changes and PET biological washout, and the PET signal was collected during irradiation (approx. 2 minutes). A dedicated computational framework was developed to compare voxel-wise PET activity distributions in the absence and in the presence of anatomical changes. This framework produced 3D discrepancy maps and enabled quantitative analysis of range shifts and morphological variations.

At 30 seconds post-irradiation, the IB-PET images from ^{11}C beams showed significantly stronger signal intensity, lower noise, and more accurately reflected dose-related range variations compared to protons or stable C-ions. The discrepancy maps derived from ^{11}C PET data accurately localized regions affected by anatomical changes, which were less clearly identified using ^{12}C or proton data.

Radioactive ion beams combined with IB-PET imaging offer substantial improvements over conventional beams by enabling real-time, high-resolution detection of anatomical and dose-related changes during irradiation. The enhanced signal quality eliminates the need for long acquisition times and could reduce the need for control CT scans.

47. Quantification of Nanoscale Free Volumes in Human Plasma Clots Using Positron Annihilation Lifetime Spectroscopy

S. Moyo^{1,2}, P. Moskal^{1,2}, E. Stepień^{1,2}

¹*Faculty of Physics, Astronomy and Applied Computer Science, Jagiellonian University, Cracow, Poland*

²*Center for Theranostics, Jagiellonian University, Cracow, Poland*

Positron annihilation lifetime spectroscopy (PALS), interpreted via the Tao–Eldrup model, provides a sensitive and quantitative method for probing nanoscopic free volumes in biological systems [1]–[4]. This study investigates free volume characteristics in human plasma blood clots under variable thermal and preparation conditions. Using ortho-positronium (o-Ps) lifetime (τ_3) and intensity (I_3), we calculated the free volume radius (R), mean free volume size (V_f), and fractional free volume (f_v) across a range of clot states.

First, we evaluated fresh plasma clots at 22°C, 37°C, and 40°C. A temperature increase from 22°C to 37°C led to a rise in τ_3 from 1.87 to 1.94 ns and in R from 0.275 to 0.282 nm, with a corresponding increase in V_f from 0.087 to 0.094 nm³ and in f_v from 0.00172 to 0.00186. These modest but consistent increases reflect enhanced molecular mobility and free volume expansion at physiological temperatures [5], [6].

At 37°C, we further compared clots in four physical states: fresh, fixed, desiccator-dried, and critical point dried. Fixed clots exhibited the highest free volume parameters ($\tau_3 = 2.03$ ns, $R = 0.290$ nm, $V_f = 0.103$ nm³, $f_v = 0.00986$), suggesting fibrin network loosening due to chemical stabilization [7]. Desiccator-dried clots showed the largest voids ($R = 0.301$ nm, $V_f = 0.114$ nm³), but with low I_3 (6%), leading to a lower effective f_v (0.00124). In contrast, critically dried clots maintained a balance between structural preservation and porosity ($R = 0.283$ nm, $f_v = 0.00683$).

These results highlight the combined impact of temperature and sample preparation methods on the nanoscale architecture of blood clots. Our findings demonstrate that positron annihilation lifetime spectroscopy (PALS) is a sensitive and reliable technique for quantifying clot porosity, with potential applications in thrombus characterization, biomaterial development, and diagnostic stratification in clinical practice [8]–[11].

[1] P. Moskal, B. Jasinska, E. Stepień, and S. D. Bass, Nat. Rev. Phys., vol. 1, pp. 527–528, 2019.

[2] S. Moyo, P. Moskal, and E. Stepień, Bio-Algorithms Med-Syst., vol. 18, no. 1, pp. 163–167, 2022.

[3] S. J. Tao, Phys. Rev. A, vol. 6, pp. 2147–2155, 1972.

[4] M. Eldrup, D. Lightbody, and J. N. Sherwood, Chem. Phys., vol. 63, pp. 51–58, 1981.

[5] Y. C. Jean, P. E. Mallon, and D. M. Schrader, *Principles and Applications of Positron and Positronium Chemistry*. Singapore: World Sci., 2003.

[6] T. Goworek et al., Chem. Phys. Lett., vol. 272, pp. 91–94, 1997.

- [7] M. Kalina et al., J. Radioanal. Nucl. Chem., vol. 322, pp. 1837–1843, 2019.
- [8] A. Shukla et al., Nat. Commun., vol. 8, p. 14798, 2017.
- [9] J. Dullius et al., Radiat. Phys. Chem., vol. 119, pp. 58–64, 2016.
- [10] Y. C. Jean, Microchem. J., vol. 42, pp. 72–102, 1990.
- [11] P. Moskal, J. Baran, S. Bass, J. Choinski, N. Chug, C. Curceanu, et al., Sci. Adv., vol. 10, p. eadp2840, 2024.



48. Towards feasibility study of Positronium yield in proton beam therapy.

W. Mryka^{1,2}, Sz. Niedźwiecki^{1,2}, E. Stępień^{1,2} and P. Moskal^{1,2}

¹ Faculty of Physics, Astronomy and Applied Computer Science, Jagiellonian University, Cracow, Poland.

² Centre for Theranostics, Jagiellonian University, Cracow, Poland.

Proton beam therapy is a quickly emerging modality of radiation treatment. Its advantages over the conventional methods - finite range, maximal energy deposition at the end of the range and low energy deposition elsewhere - provide more conformal dose distribution over the tumor, save surrounding tissues and make the therapy more comfortable for the patient. However, to make an efficient use of those advantages one needs to develop a beam range monitoring system. Since the possible solution is utilizing the PET system for monitoring purposes, another curious possibility emerges [1,2,3]. A PET system (the J-PET system in particular) enables positronium life-time measurements in PET imaging for diagnostics [4,5,6]. The same information about positronium life-time can be obtained also during proton beam therapy. However, this information is more difficult to acquire due to the high background coming from prompt gamma radiation, various isotopes that emit positrons and other particles and the medium that affects the life-time. Developing the methods for enabling positronium studies in proton beam therapy is crucial for determination of hypoxia level in the tissues, especially in the tumor region. Hypoxic tissues are more resistant to radiation therapy than normoxic tissues. Hence, determining the oxygenation level tumor and surrounding tissues would enhance the effectiveness of the therapy [7,8]. In this work we study the feasibility to utilize the J-PET system to conduct positronium studies in proton beam therapy. Estimation of the β^+ - emitting isotope production rate during irradiation will be presented together with positronium yield and efficiency of the positronium signal registration with the J-PET system in dual-head configuration.

[1] K. Parodi, T. Yamaya, and P. Moskal, Z. Med. Phys., vol. 33, pp. 22–34, 2023.

[2] M. Durante and J. Loeffler, Nat. Rev. Clin. Oncol., vol. 7, pp. 37–43, 2010.

[3] C. Graeff, L. Volz, and M. Durante, Prog. Part. Nucl. Phys., vol. 131, p. 104046, 2023.

[4] P. Moskal et al., Sci. Adv., vol. 10, p. eadp2840, 2024.

[5] P. Moskal et al., Phys. Med. Biol., vol. 64, no. 5, p. 055017, 2019.

[6] P. Moskal et al., Sci. Adv., vol. 7, no. 42, 2021.

[7] P. Moskal and E. Ł. Stępień, Bio-Algorithms Med-Syst., vol. 17, no. 4, pp. 311–319, 2021.

[8] P. Moskal, B. Jasińska, and E. Ł. Stępień, Nat. Rev. Phys., vol. 1, pp. 527–529, 2019.

49. Mirror matter : towards precise measurement of orthopositronium lifetime

Justyna Medrala-Sowa¹, Pawel Moskal^{1,2}, Elena Perez del Rio^{1,2}

¹ *Faculty of Physics, Astronomy and Applied Computer Science, Jagiellonian University, Cracow, Poland.*

² *Centre for Theranostics, Jagiellonian University, Cracow, Poland.*

Positronium (Ps) is an exotic atom composed of an electron and its antiparticle, the positron, bound together in a short-lived quantum system. This bound state serves as a unique system for probing fundamental physics, as its properties are precisely predicted by Quantum Electrodynamics (QED) within the Standard Model (SM). Furthermore, its decay processes, which are effectively modeled using Monte Carlo simulations, provide valuable information on various domains of particle physics.

At the Jagiellonian University, the J-PET detector (Jagiellonian Positron Emission Tomograph), a novel tomography system based on plastic scintillator detectors, has been developed [1]. This setup offers high angular and timing resolutions [2-4], enabling multidisciplinary studies of positronium decays. Therefore, it is possible to measure the lifetime of positronium with high precision with J-PET.

In this work, we report on ongoing searches for Dark Matter signatures in ortho-positronium

(o-Ps) decays using the J-PET detector. The primary objective is to explore the existence of Mirror Matter, a hypothetical form of matter proposed to restore parity symmetry and considered a plausible candidate for the Dark Matter component of the Universe. Our study aims to refine current experimental limits by achieving high-precision measurements of the o-Ps lifetime in its three-photon decay channel, comparing these results with QED predictions to search for potential deviations that could be interpreted as a signal of the presence of Dark Matter [5].

We acknowledge support from the National Science Centre of Poland through Grants No. 2019/35/B/ST2/03562, 2020/38/E/ST2/00112 and the SciMat and qLife Priority Research Area budget under the auspices of the program Excellence Initiative-Research University at Jagiellonian University.



50. Prospects for Positronium and Quantum Entanglement Imaging with J-PET

P. Moskal^{1,2}


¹ *Faculty of Physics, Astronomy and Applied Computer Science, Jagiellonian University, Cracow, Poland.*

² *Centre for Theranostics, Jagiellonian University, Cracow, Poland.*

Jagiellonian-PET (J-PET) is a novel, cost-effective positron emission tomography technology based on plastic scintillators [1,2]. The J-PET system constructed at the Jagiellonian University is the first multi-photon PET scanner [3] capable of measuring momentum vectors and the orientation of polarization planes of photons originating from positronium decays [4]. Positronium imaging is a newly invented method for imaging the properties of positronium in living organisms [5,6,7,8]. Quantum Entanglement Imaging is a method enabling the imaging the degree of the entanglement of annihilation photons [6].

We will present the first-ever images of the properties of positronium in humans [8], the first multi-photon images from the decays of positronium atoms into three photons [3], and the first observation of non-maximal entanglement of photons from positronium annihilation in matter [9]. We will discuss the status of the development of (i) positronium imaging and (ii) degree of quantum entanglement imaging as possible diagnostic biomarkers of tissue pathology [10] and biomarkers of hypoxia [11]. We will also discuss the possibility of developing a method for studies of material properties by the measurement of the degree of quantum entanglement of annihilation photons.

- [1] P. Moskal, E. Ł. Stępień, PET Clinics 15, 439, 2020
- [2] P. Moskal et al., Phys. Med. Biol. 66, 175015, 2021
- [3] P. Moskal et al., Nature Communication 12, 5658, 2021
- [4] P. Moskal et al., Nature Communication 15, 79, 2024
- [5] P. Moskal, Positronium Imaging, IEEE NSS MIC 2018, 10.1109/NSSMIC.2018.8824622
- [6] P. Moskal et al., Nature Reviews Physics 1, 527, 2019
- [7] P. Moskal et al., Science Advances 7, eabh4394, 2021
- [8] P. Moskal, ..., E. Ł. Stępień, Science Advances 10, eadp2890, 2024
- [9] P. Moskal et al., Science Advances 11, eads3046, 2025
- [10] P. Moskal, ..., E. Ł. Stępień, EJNMMI Phys. 10, 22, 2023
- [11] P. Moskal, E. Ł. Stępień, Bio-Algorithms and Med-Systems 17, 311, 2021

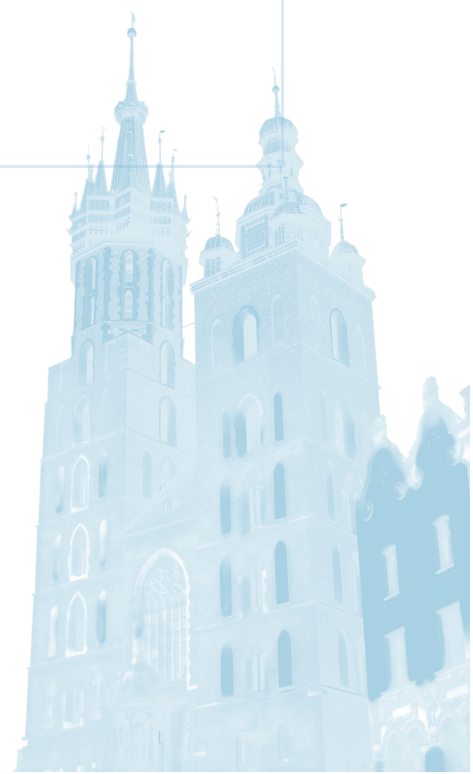

51. Enhancement of Biological PET Imaging via Quantum Entanglement using GAGG-SiPM pixel ring detectors

Koki Nakamura¹, Mizuki Uenomachi², Pietro Caradonna¹, Kei Kamada³, Macoto Fujimoto¹

¹*The University of Tokyo, Japan*

²*Institute of Science Tokyo, Japan*

³*Tohoku University, Japan*

Exploiting the quantum entanglement of the annihilation γ -pair and deliberately inducing a second Compton interaction in each detector could furnish additional observables that enable more effective separation of true coincidences, thereby improving the signal-to-background ratio. A small-animal prototype PET / quantum-entangled PET system has been developed with three rings, each comprising eight 8×8 GAGG-SiPM pixel detectors whose pixel pitch is 3.2 mm. Pixel-level energy is derived from pulse-width measurements calibrated with standard sources such as Am-241 and Ba-133, and all energy-and-timing information is recorded in list mode to extract both photo-absorption and Compton events. The image quality of a phantom obtained with standard PET (utilizing two photo-absorption events) and with quantum-entangled PET (utilizing two Compton events) is evaluated visually and quantitatively by standard metrics including contrast-to-noise ratio, recovery coefficient, and spatial resolution. These results will be compared with Geant4-based simulation outputs to assess any discrepancies, and the first trial outcome of in-vivo small-animal imaging will also be presented.



52. Range Monitoring in Proton Therapy Using the J-PET Scanner: First Experimental Insights

Szymon Niedźwiecki^{1,2}, Antoni Rucinski³, Jan Gajewski³, Jakub Baran^{1,2},
Grzegorz Korcyl^{1,2}, Damian Borys⁴, Karol Brzeziński³, Paulina Stasica³,
Pawel Moskal^{1,2}

¹ *Faculty of Physics, Astronomy and Applied Computer Science, Jagiellonian University, Cracow, Poland.*

² *Centre for Theranostics, Jagiellonian University, Cracow, Poland.*

³ *Institute of Nuclear Physics Polish Academy of Sciences, Cracow Poland*

⁴ *Silesian University of Technology, Biotechnology Centre, Katowice, Poland*

A method for experimental determination of the proton beam range in a water-equivalent phantom using the modular J-PET detector is presented. A series of $4 \times 4 \times 4$ cm³ dose volumes were irradiated with proton beams delivering uniform doses at varying penetration depths with 16 Gy dose. Data acquisition was performed using a dual-head configuration of the J-PET prototype, with each head consisting of three layers of four detection modules. The system operated in a triggerless acquisition mode during and after irradiation. For image reconstruction, only data collected in the post-irradiation period were utilized, employing the CASToR framework.

The reconstructed PET images represented spatial distributions of emitters produced by nuclear interactions of protons within the phantom. Activity profiles were extracted and fitted with a sigmoidal function to determine the range of activity distributions for each irradiated field. A linear correlation was observed between the simulated dose ranges and those derived from PET data. Lower doses were investigated by randomly rejecting part of the data sample. For 4 Gy dose, the mean range shift error was approximately 1 mm for a 5-minute acquisition window and decreased to below 1 mm when 30 minutes of post-irradiation data were used. These results indicate the feasibility of precise proton range verification using the J-PET system.



53. Targeted radioligand therapy

Marta Opalińska

*Department of Endocrinology, Jagiellonian University Collegium Medicum,
Cracow, Poland*

Targeted radioligand therapy (RLT) involves the administration of a radiopharmaceutical—an agent composed of an α or β -emitting radionuclide bound to a molecule that selectively targets specific receptors on tumor cells. RLT is already considered the gold standard for the treatment of neuroendocrine tumors (NETs) and prostate cancer. However, an increasing number of early clinical trials are demonstrating its potential benefits in the treatment of other selected cancers.

In the case of NETs, RLT improves progression-free survival and helps control hormone secretion in functioning tumors, while generally causing relatively mild toxicity. The current standard of care involves administering fixed doses of radiopharmaceuticals over four treatment cycles. However, growing evidence suggests that treatment outcomes—in terms of both efficacy and toxicity—are closely related to the actual radiation dose delivered.

The fixed administered activity can result in a wide range of absorbed doses in tumors and healthy tissues, due to patient-specific metabolic differences and tumor heterogeneity. Therefore, the absorbed dose, rather than the administered activity, plays a critical role in determining treatment response. As a result, a one-size-fits-all approach—whether using a fixed or weight-adjusted dose—can easily lead to under-treatment or over-treatment, the latter increasing the risk of toxicity.

Dosimetry offers a way to optimize the efficacy of RLT and tailor treatment to individual patients. Unfortunately, performing full dosimetry requires at least four post-treatment imaging sessions along with extensive data processing, making it time-consuming and resource-intensive for medical staff.

We will discuss the available evidence to assess how dosimetry influences the treatment process and whether its effectiveness justifies the additional time and effort required.

[1] P. Moskal, E. Stępień, J. Baran et al., Sci. Adv., vol. 7, p. eabh4394, 2021.

[2] F. Tayefi, P. Moskal, E. Stępień et al., Bio-Algorithms Med.-Syst., vol. 19, pp. 133–139, 2023.

[3] P. Moskal, E. Stępień, J. Baran et al., Sci. Adv., vol. 10, p. adp2840, 2024.

[4] P. Moskal, E. Stępień, PET Clinics, vol. 15, no. 4, pp. 439–452, 2020.

[5] W. Krzemień, P. Moskal, E. Stępień et al., Acta Phys. Pol. B, vol. 51, p. 165, 2020.

54. Probing nuclear structure using lifetime measurements

R. Palit

Tata Institute of Fundamental Research, Mumbai, India

Level lifetime measurements are crucial in nuclear structure studies to identify isomers and probe the different excitation phenomena in nuclei. The Digital INGA setup at TIFR [1] has been upgraded [2,3] with an array of LaBr_3/Ce scintillator detectors in addition to the Compton-suppressed HPGe Clover detectors. Experiments have been conducted to probe the evolution of octupole collectivity in La and Zr isotopes [4,5] and the structure of a doubly odd ^{138}La isotope. The lifetime measurements in ^{88}Sr confirms the existence of an attractive shears between two particle blades for the first time in any nuclei [6]. Some of the results from these experiments, covering diverse aspects of nuclear structure near $N=50$ and 82 neutron shell gap will be presented.



55. Towards the development of an iterative algorithm for positronium lifetime imaging using ^{44}Sc with the modular J-PET

Anand Pandey^{1,2}, Sushil Sharma^{1,2}, Manish Das^{1,2}, Hsin-Hsiung Huang³, Berkin Uluutku³, Giuliano Gasparato³, Chien-Min Kao⁴, Ewa Stepień^{1,2}, Pawel Moskal^{1,2}

¹*Faculty of Physics, Astronomy and Applied Computer Science, Jagiellonian University, Cracow, Poland*

²*Centre for Theranostics, Jagiellonian University, Cracow, Poland.*

³*Department of Statistics and Data Science, University of Central Florida, Orlando, USA*

⁴*Department of Radiology, University of Chicago, Chicago, USA*

Positronium Lifetime Imaging (PLI) represents an emerging imaging modality which enhances PET capabilities through its ability to map the spatial distribution of mean lifetimes of positronium atoms (Ps) [1,2,3]. The high sensitivity of Ps lifetime, particularly of the ortho-Ps (a triplet state of Ps), to nano-scale environments makes PLI a promising tool for studying tissue microstructure and pathological behavior at scale non accessible by standard PET [4,5]. We aim to develop a PLI method using the ^{44}Sc radioisotope, which has a clinically favorable profile featuring a suitable half-life (4.04 h) [6], a high branching ratio of positron emission ($\sim 94.3\%$), and the emission of a 1157 keV prompt gamma photon [7,8]. PLI is based on the registration of three coincident photon events, where the annihilation position is reconstructed using the two 511 keV annihilation photons, while the prompt gamma provides the start signal for the formation of ortho-Ps [1,3].

In this work, we report the results from a recent study using the NEMA IQ phantom with the Modular J-PET. Out of the six spheres of the phantom, the three largest spheres were filled with ^{44}Sc , and the remaining three with ^{18}F , diluted with water such that the activity concentration ratio at the beginning of the experiment was 1:3 [8]. The analysis algorithm was developed primarily to reconstruct the PLI for the spheres filled with ^{44}Sc [9].

The data were analyzed using the J-PET data analysis framework. We studied only those events in which two annihilation photons (511 keV) are in coincidence with the prompt gamma (1157 keV). For each event, the hit positions of both annihilation photons were used to define the Line of Response (LOR), which was processed using Siddon's ray-tracing algorithm to determine the voxel-wise intersections [10]. The Maximum Likelihood Expectation Maximization (MLEM) algorithm [11] is used to reconstruct the activity concentration image iteratively. The difference between the average registration time of the annihilation photons and the prompt gamma was used to compute the lifetime, which was then sorted voxel-wise to construct the lifetime histogram. The mean Ps lifetimes were then extracted from the histograms for lifetime imaging.

As a next step, we aim to integrate lifetime estimation directly into the iterative process [8], enabling simultaneous reconstruction of activity and lifetime images within a unified MLEM framework.

In this presentation, we will show the results obtained using Siddon's ray-tracing and MLEM reconstruction, and briefly discuss the plans to incorporate lifetime information to obtain positronium lifetime images.

- [1] P. Moskal, Proc. IEEE Nucl. Sci. Symp. Med. Imaging Conf. (NSS/MIC), p. 1, 2019.
- [2] P. Moskal et al., IEEE Trans. Radiat. Plasma Med. Sci., in press, 2025.
- [3] P. Moskal et al., Sci. Adv., vol. 10, p. eadp2840, 2024.
- [4] P. Moskal et al., EJNMMI Phys., vol. 10, p. 22, 2023.
- [5] S. D. Bass et al., Rev. Mod. Phys., vol. 95, p. 021002, 2023.
- [6] M. T. Durán et al., Appl. Radiat. Isot., vol. 190, p. 110507, 2022.
- [7] P. Moskal and E. Stępień, PET Clin., vol. 15, p. 439, 2020.
- [8] M. Das et al., arXiv:2506.07230, 2025.
- [9] H. H. Huang et al., IEEE Trans. Radiat. Plasma Med. Sci., vol. 9, p. 478, 2025.
- [10] R. L. Siddon, Med. Phys., vol. 12, p. 252, 1985.
- [11] L. A. Shepp et al., IEEE Trans. Med. Imaging, vol. 1, p. 113, 1982.



56. Feasibility study of Antihydrogen vertex imaging using the modular J-PET

Piyush Pandey^{1,2}, Sushil Sharma^{1,2}, Pawel Moskal^{1,2}, Anoop Kunimmal Venadan^{1,2}, Grzegorz Korcyl^{1,2}, Krzysztof Kacprzak^{1,2}

¹*Faculty of Physics, Astronomy and Applied Computer Science, Jagiellonian University, Cracow, Poland*

²*Centre for Theranostics, Jagiellonian University, Cracow, Poland.*

The Antihydrogen Experiment: gravity, Interferometry, Spectroscopy (AEGIS) at CERN aims to measure the gravitational acceleration of antihydrogen atoms to test the Weak Equivalence Principle for antimatter systems [1,2]. The antihydrogen beam is produced through a charge exchange reaction between Rydberg-excited positronium and antiprotons, which subsequently passes through a moiré deflectometer equipped with two precisely spaced gratings [3,4,5]. An accurate beam profile monitoring is essential to quantify the spatial characterization of antihydrogen beam for the precision of gravitational measurements [6]. The beam profile can be assessed by tracking the high energetic pions produced during the interaction of antihydrogen atoms with grating materials as they traverse through the deflectometer. To achieve this, J-PET collaboration is developing state-of-art detection modules [7,8,9]. In the planned experiment, two pairs of J-PET detection modules will be used to span the full axial length of moiré setup [10], complementing the existing detection systems [6,11]. The generated pions, being minimum ionizing particles (MIPs), are expected to travel in approximately straight trajectories while depositing characteristic energy in the scintillators. Their paths can be tracked through consecutive registrations in any two detectors of each J-PET module pair. The hit positions in these modules enable the reconstruction of individual pion trajectories, which are then back-projected to estimate the spatial coordinates of the annihilation vertex.

A customized Geant4 simulation application was developed to model the realistic generation of charged pions, originating from antihydrogen annihilations, as well as their propagation to J-PET modules for detection. An analysis algorithm was also developed based on the back-projection technique to image the annihilation vertices. In this presentation, results from the feasibility studies will be presented and discussed.

Acknowledgments: We acknowledge the support from the National Science Centre of Poland through Grants No. 2019/35/B/ST2/03562, 2021/42/A/ST2/00423, 2021/43/B/ST2/02150, 2023/50/E/ST2/00574 and the SciMat and qLife Priority Research Area budget under the program Excellence Initiative—Research University at Jagiellonian University.

[1] M. Doser et al., Class. Quantum Grav., vol. 29, p. 184009, 2012.

[2] S. G. Karshenboim, J. Phys. B: At. Mol. Opt. Phys., vol. 49, p. 144001, 2016.

- [3] C. Amsler et al., Commun. Phys., vol. 4, p. 19, 2021.
- [4] S. Aghion et al., Nat. Commun., vol. 5, p. 4538, 2014.
- [5] L. Gloggler et al., Phys. Rev. Lett., vol. 132, p. 083402, 2024.
- [6] M. Berghold et al., Sci. Adv., vol. 11, p. 14, 2025.
- [7] P. Moskal et al., Sci. Adv., vol. 10, p. eadp2840, 2024.
- [8] P. Moskal et al., Nat. Commun., vol. 15, p. 78, 2024.
- [9] S. Sharma et al., Nucl. Instrum. Meth. A, vol. 1062, p. 169192, 2024.
- [10] R. C. Ferguson et al., J. Phys. Conf. Ser., vol. 3029, p. 012005, 2025.
- [11] P. Conte et al., arXiv:2506.09274v1, 2025



57. Development of Advanced PET Technology for Scientific and Clinical Applications

Qiyu Peng

ShenZhen Bay Laboratory, Shenzhen, China

Positron Emission Tomography (PET) is playing an increasingly critical role in biomedical research and clinical diagnostics, particularly in the fields of oncology, neurology, and cardiology. In this talk, I will introduce the recent progress from the Advanced Molecular Imaging Laboratory (AMIL) at Shenzhen Bay Laboratory, including innovations in high-resolution small-animal PET systems, brain-dedicated and cardiac-dedicated PET systems, wearable brain PET for both preclinical and human use, and the development of a 2-meter total-body TOF-DOI PET/CT system. I will also highlight strategies for translating these technologies into clinical applications to address unmet needs in precision medicine and global health. In this context, international joint effort is not only beneficial but essential, and it is the only viable path toward achieving truly affordable molecular imaging solutions for global health.



58. Para-positronium and beyond: probing two-photon annihilation in bound states

Milena Piotrowska, Francesco Giacosa

Jan Kochanowski University, Kielce, Poland

We investigate two-photon annihilation processes in neutral pseudoscalar bound states, focusing on para-positronium, the charmonium state $c(1S)$ and the bottomonium state $b(1S)$, within a QFT framework that implements the Weinberg's compositeness condition. . By evaluating triangle loop diagrams with constituent fermions ((anti)electrons in positronium and (anti)quarks in $c(1S)$ and $b(1S)$), we compare QED and QCD bound states. As additional applications, we evaluate the weak decay constants for both QED and QCD bound states, as well as rare positronium processes: the decay into one photon and two neutrinos and the possible mixing with the 'putative' axial-vector $X(17)$ particle.



59. Extracellular vesicle flow cytometry: what's possible and what's next

Edwin van der Pol^{1,2}

¹Biomedical Engineering & Physics, Amsterdam UMC, University of Amsterdam, Biomedical Engineering & Physics, Amsterdam, The Netherlands

²Laboratory of Experimental Clinical Chemistry, Amsterdam UMC, University of Amsterdam, Laboratory of Experimental Clinical Chemistry, Laboratory Specialized Diagnostics & Research, Department of Laboratory Medicine, Amsterdam, The Netherlands

Extracellular vesicles (EVs) are increasingly recognized as mediators of intercellular communication and hold promise as disease biomarkers and therapeutic agents. Among available techniques, flow-based methods currently remain the only approach capable of quantifying EV concentrations - i.e. the absolute number of submicrometer, immunostained particles per milliliter of fluid - in a reproducible, standardized and practical manner. Nevertheless, detecting EVs with flow cytometry presents unique challenges.

In this talk, I will provide an overview of the capabilities and limitations of EV flow cytometry, based on our work at the Amsterdam Vesicle Center (vesiclecenter.com). Key topics will include: (1) detection sensitivity, addressing the challenges in distinguishing EVs from background noise, (2) standardization and calibration, discussing the importance of signal calibration to ensure reproducible experiments, (3) the dilution paradox, addressing assay design considerations for measurements on EVs in blood plasma, and (4) advancements in instrumentation, highlighting recent technological developments that enhance single-EV detection.

By examining these areas, I aim to delineate what is currently achievable with EV flow cytometry and identify avenues for future research and technological innovation.

60. μ PPET, a J-PET application for cosmic rays investigation

Alessio Porcelli^{1,2,3}

¹Faculty of Physics, Astronomy and Applied Computer Science, Jagiellonian University, Cracow, Poland

²Centro de Investigación, Tecnología, Educación y Vinculación Astronómica, Universidad de Antofagasta Chile

³Laboratori Nazionali di Frascati, Istituto Nazionale di Fisica Nucleare, Via Enrico Fermi 54, 00044 Frascati, Italy

The J-PET machines at Jagiellonian University are advanced scintillator systems capable of precisely detecting particle positions. While designed to be a tomographer, they can also detect cosmic rays, especially muons. In fact, these particles are often considered background noise. However, reversing this perspective, J-PET can be used to study particles originating from air showers induced by cosmic rays. Notably, J-PET enables the study of air shower muons, which are crucial for identifying the atomic mass of primary cosmic rays.

Nevertheless, the current challenge lies in the hadronic interaction models correctly linking muon density at ground level to the mass of cosmic rays—the longstanding 15-year Muon Puzzle, for which the models predict far fewer muons compared to reality. In this talk, we will show how J-PETs can investigate the Muon Puzzle, particularly by testing a new hypothesis aimed at solving it.



61. Cold Neutron Interferometry for Fundamental Physics Experiments

Luca Povolo, Philipp Heil, Gjon Markaj, Jakob Micko, Marc Persoz, Ciro Pistillo, Florian M. Piegsa

Laboratory for High-Energy Physics and Albert Einstein Center for Fundamental Physics, University of Bern, Switzerland

In the Fundamental Neutron and Precision Physics Group at the University of Bern, we are using cold and ultracold neutrons for fundamental physics research. In particular, we are interested in the neutron electric charge. Currently, the best measurement of the charge is $(-0.4 \pm 1.1) \times 10^{-21}e$, where e is the elementary electric charge [1].

With the goal of improving this result, the group developed a novel high-visibility Talbot-Lau interferometer for cold neutron beams using absorption gratings with microscopic dimensions [2-3]. The apparatus consists of three gratings. The neutrons pass through the first two gratings and create an interference pattern at the position of the last. This pattern contains information of a potential force acting on the beam perpendicular to the interferometer path. By applying a strong electric field between the gratings, the possible electric force acting on the neutrons is measured by comparing the pattern formed for opposite electric field directions [3].

Detailed measurements with a prototype version of the apparatus have been performed successfully at the Institute Laue-Langevin (Grenoble, France) [3]. Presently, we are working on improvements for the construction of a final apparatus that would let us reach or even surpass the previous best limit on the neutron electric charge. To conduct systematic investigations, we built an approximately 1-meter-long scaled-down version of the interferometer. In this talk, we will present the status of the experiment, describe the operation and show first results obtained with the scaled-down Talbot-Lau interferometer.

[1] J. Baumann et al., Phys. Rev. D, vol. 37, p. 3107, 1988.

[2] F. M. Piegsa, Phys. Rev. C, vol. 98, p. 045503, 2018.

[3] M. Persoz, Ph.D. dissertation, 2024.



62. Development of high-Z organic scintillators for modern SPECT imaging and theranostic dosimetry

Flaminia Quattrini¹, Mattia Bonuso², Alberto Burattini³, Marina Carruezzo⁴, Maria Silvia De Feo⁵, Angelica De Gregorio⁶, Giuseppe De Vincentis⁷, Gaia Franciosini³, Viviana Frantellizzi⁷, Marco Garbini², Leonardo Gasparini⁸, Nils Krah, Marco Magi³, Enrico Manuzzato⁸, Michela Marafini², Leonardo Mattiello³, Roberto Passerone¹⁰, Vincenzo Patera³, Daniele Rocco³, Alessio Sarti³, Angelo Schiavi³, Marco Toppi³, Samane Vahidi¹⁰, Arianna Vannucci², Giacomo Traini⁶

¹Department of Physics, University of Rome "La Sapienza", Rome, Italy

²"Enrico Fermi" Historical Museum of Physics and Study & Research Centre (CREF), Rome, Italy

³Sapienza University of Rome, Department of Basic and Applied Sciences for Engineering, Rome, Italy

⁴National Center for Radiation Protection and Computational Physics, Italian National Institute of Health, Rome, Italy

⁵Department of Radiology, Oncology and Anatomo-Pathology, University of Rome "La Sapienza", Rome, Italy

⁶National Institute for Nuclear Physics (INFN), Roma I Section, Rome, Italy

⁷Department of Radiology, Oncology and Anatomo-Pathology, Sapienza University of Rome, Rome, Italy

⁸FBK - Sensors and Devices, IRIS Research Unit, Povo (TN), Italy

⁹University of Lyon, Center for Research in Image Acquisition and Processing for Health, Lyon, France

¹⁰University of Trento, Department of Information Engineering and Computer Science, Povo (TN), Italy



In the fight against cancer, improving the detectors performance is crucial to enhance diagnostic accuracy and optimize therapies. Current clinical SPECT systems predominantly rely on NaI(Tl) crystals, which, despite their advantages, suffer from limited count-rate due to long scintillation decay times. Our goal is to address this limitation by developing an innovative class of plastic scintillators doped with high-Z elements. These materials combine the fast timing characteristics of organic scintillators with improved gamma-ray detection efficiency via enhanced photoelectric interaction probability.

Our research focused on synthesizing novel organic fluorophores to fabricate plastic scintillators doped with various high-Z elements—including Bismuth, Cerium, Lead and Erbium—with concentrations up to 10%. The resulting prototypes show promising characteristics in terms of optical transparency, dopant homogeneity, light yield and timing performance, reaching levels comparable with commercial standards. Moreover, we explored different fabrication techniques, including polymerization inside molds of different materials (PE, PTFE, metal) and the use of 3D-printed resin as a scintillator substrate.

These novel detectors are at the core of two parallel projects. The first one involves the development of a next-generation SPECT detector, in which the doped scintillators are polymerized directly into the holes of a 3D-printed tungsten matrix that also serves as a collimator, with signal readout performed by tiled CMOS sensors to ensure optimal temporal resolution and system modularity. Additionally, FPGA matrices will be mounted on the back of the detector to perform data pre-processing. The second project aims at designing a compact portable dosimeter tailored for metastatic castration-resistant prostate cancer (mCRPC) patients undergoing Lu-177-PSMA-617 radio-metabolic therapy. The device is designed to retrieve the radiopharmaceutical washout curve without requiring multiple SPECT scans, which is crucial for patients experiencing pain or mobility limitations. The goal is the determination of the patient-specific radiometabolic parameters to customize the prescription, thus optimizing the effectiveness of the therapy.



63. High-Resolution Intravital Imaging: Novel On-Chip PET and iQID Camera for Personalized Radiopharmaceutical Therapy and Microdosimetry

Narendra Radhod

University of Bern, Switzerland

Advances in microdosimetry and personal radiopharmaceutical therapy necessitate imaging devices able to capture functional and molecular processes at cellular and sub-organ length scales with high spatial resolution and sensitivity. This article presents a two-platform approach to high-resolution intravital imaging using two new devices: an On-Chip Positron Emission Tomography (PET) scanner and an enhanced ionising radiation Quantum Imaging Detector (iQID) camera.

On-Chip PET is developed specifically for Organ-On-Chip (OOC) imaging, with monolithic LYSO crystals and multi-surface silicon photomultiplier (SiPM) readouts. A CNN trained on Monte Carlo simulation data enabled accurate gamma-ray interaction point determination. Initial experiment results yielded a spatial resolution of approximately 0.55 mm, validated by imaging of a fluorine-18 (^{18}F) point-source grid. These results validate the system's capability for integration of functional molecular imaging into microphysiological platforms. First experimental results with real data will be presented for both point-like sources, demonstrating the system's capability in realistic imaging scenarios.

In addition, the high-resolution iQID camera system with a 2048×2448 pixel array was evaluated using ^{177}Lu -labelled and ^{18}F -labelled phantom / biological material. Systematic optimization of acquisition parameters and advanced Python-based analysis supplemented with machine learning enabled precise event localisation, radiotracer imaging, and real-time particle discrimination (alpha, beta and gamma). The iQID system was demonstrated to operate robustly for quantitative digital autoradiography with sub-millimeter accuracy.

Together, these tools constitute a strong preclinical radiopharmaceutical testing arsenal enabling high-resolution visualization of radiotracer distribution and radiation interaction. Combined, their potential offers new avenues for personalized therapy planning, drug discovery, and cell-level dosimetry in nuclear medicine

64. Optimizing the event selection of the total-body J-PET scanner with a brain PET insert: a simulation study

M. Rädler^{1,2} and P. Moskal^{1,2} for the J-PET collaboration

¹Faculty of Physics, Astronomy and Applied Computer Science, Jagiellonian University, Cracow, Poland

²Centre for Theranostics, Jagiellonian University, Cracow, Poland.

The J-PET collaboration (Jagiellonian positron emission tomography) is working towards the realization of a large field-of-view (FOV) total body J-PET (TB-J-PET) scanner enabling, among others, low dose imaging, short scan times, and dynamic imaging. The key distinctive feature, i.e., the utilization of cost-effective plastic scintillators, could facilitate a wider adoption of large FOV scanners. Simultaneously, dedicated brain PET imaging has shown various exciting applications, hence we are currently studying the combination of the TB-J-PET with a brain PET insert via Monte Carlo simulations. In previous works, we investigated the performance characteristics of different geometries, such as a frontal detector versus a cylindrical insert or different plastic scintillator dimensions. In addition to sensitivity, spatial resolution was investigated via MLEM reconstructions of the Derenzo phantom.

In this work, we focus on the impact of more realistic event selection, taking into account temporal and spatial resolution limits. For this purpose we employ the software package GATE v9.4.1, enabling multi-detector geometries (including in-house corrections of the Compton interactions). Generally, PET imaging with plastic scintillators suffers from a significant background of scattered events among the detectors. In order to identify and suppress them, a scatter test is usually performed, excluding coincidences that are light-like. However, brain PET detectors are placed much closer to the patients (to decrease uncertainties from non-collinearity of the annihilation photons), so that under finite time resolution, one cannot distinguish scattered from real events. Secondly, previous simulation studies have relied on a lower energy deposition cut of 200 keV for both events in a coincidence. However, we show that this choice is sub-optimal leading to a higher percentage of incorrectly identified coincidences. After sorting the events into multiplicity groups, we propose an alternative time-based event selection, taking advantage of the excellent time resolution of plastic scintillators. We provide an in-depth quality analysis together with a comparison to an energy-based event selection.

65. Characterization of optical photon transport in Long Plastic Scintillators

Sushil Sharma^{1,2}, Neha Gupta³, Sumit Kundu^{1,2}, Anoop Kunimmal Venadan^{1,2},
Lukasz Kaplon^{1,2}, Pawel Moskal^{1,2}

¹*Faculty of Physics, Astronomy and Applied Computer Science, Jagiellonian University, Cracow, Poland*

²*Centre for Theranostics, Jagiellonian University, Cracow, Poland*

³*Department of Physics, Dyal Singh College, University of Delhi, India*

Plastic scintillators have long been used in nuclear and particle physics experiments as cost-effective detectors [1]. The longer attenuation length for light transmission makes them ideal for applications requiring a larger field-of-view (FOV) [2]. The Jagiellonian PET (J-PET) collaboration has pioneered their use to build the first plastic scintillator-based PET scanner, which is composed of 50 cm long plastic scintillators [3,4]. With the successful demonstration of modules constructed based on J-PET technology in both medical [5,6] and fundamental physics [7,8,9,10], the collaboration now aims to construct standalone detection modules using even longer scintillators. Since light propagation in long plastic scintillators depends strongly on the interaction position and direction, it is required to perform a thorough study on scintillator light yield, light attenuation during the transport along the strip, variation in the time of detected photons, and how uniformly the light is collected [11]. Furthermore, the influence of surface reflectivity also plays a crucial role in shaping the detector response [12]. All these characteristic properties of the scintillator directly impact both the timing and spatial resolution [13], which are key parameters to optimize the overall performance, particularly when signals are read out only from the ends of the scintillator.

We have developed a Monte Carlo-based simulation package in Geant4 to characterize optical photon transport in plastic scintillators of various sizes [14]. The simulated results will be validated against experimental data to ensure reliability and accuracy. In this presentation, we will discuss the structure of the developed package and present the results obtained from the simulations.

- [1] B. Seitz, JINST, vol. 7, p. C01031, 2012.
- [2] L. Kaplon et al., Nucl. Instrum. Meth. A, vol. 1051, p. 168186, 2023.
- [3] P. Moskal et al., Acta Phys. Polon. B, vol. 47, p. 509, 2016.
- [4] S. Niedźwiecki et al., Acta Phys. Polon. B, vol. 48, p. 1567, 2017.
- [5] P. Moskal et al., Sci. Adv., vol. 7, p. eabh4394, 2021.
- [6] P. Moskal et al., Sci. Adv., vol. 10, p. eadp2840, 2024.
- [7] P. Moskal et al., Nat. Commun., vol. 12, p. 5658, 2021.
- [8] P. Moskal et al., Physics, vol. 17, p. 138, 2024.
- [9] P. Moskal et al., Nat. Commun., vol. 15, p. 78, 2024.
- [10] P. Moskal et al., Sci. Adv., vol. 11, p. eads3046, 2025.
- [11] M. Gierlik et al., Nucl. Instrum. Meth. A, vol. 593, p. 426, 2008.
- [12] A. Taheri et al., Measurement, vol. 97, p. 100, 2017.
- [13] P. Moskal et al., Phys. Med. Biol., vol. 61, p. 2025, 2016.

66. Direct three gamma positronium imaging and cascade gamma chemical imaging

Kenji Shimazoe

The University of Tokyo, Japan

Nuclear medical imaging devices, PET and SPECT, are powerful and highly sensitive to the accumulation of molecules with a small amount of radio-nuclides. Extracting physicochemical micro-environmental information in addition to accumulation could contribute to more accurate diagnosis and therapy in radio-theranostics. A novel direct imaging technique of three gamma decays from ortho-positronium together with two gamma decays for quantifying the $3g/2g$ ratio indicating oxygen concentration and void size in PET device, as well as the cascade gamma-ray sensing of pH with In-111 nuclides in SPECT device will be discussed in the presentation.



67. Scientific Computing: Remote Access, CNN Segmentation, and SARS-CoV-2 Dynamics

Udai Singh

Deutsches Elektronen-Synchrotron (DESY), Germany

This work presents an integrated application of scientific computing spanning cloud-based experimental control, biomedical image segmentation, and mathematical modeling of viral infection.

We begin with the deployment of a remote access infrastructure at DESY Photon Science that enables secure, scalable, and distributed beamline experiment control. This platform integrates Kubernetes clusters, Nomad, and Consul for orchestration and dynamic service discovery, with Traefik providing secure HTTP routing. The architecture ensures high availability, flexibility, and streamlined access for remote scientific workflows.

In biomedical imaging, we address the segmentation of knee osteoarthritis (OA) in MRI scans. We compare convolutional neural networks (CNNs) with Gaussian mixture modeling (GMM) as segmentation techniques. Masks are generated using the napari framework with preprocessing steps including thresholding, Gaussian blur, and image registration with ANTs. This approach enhances anatomical localization and supports robust segmentation of degenerated cartilage regions.

Lastly, we introduce a stochastic model of early SARS-CoV-2 infection, focused on the regulation of viral transcription. The model uses experimental data from early infection time points and captures the dynamics of transcription-translation conflict, particularly in discontinuous transcription events. This computational framework serves as a tool for identifying potential therapeutic targets in the early stages of viral replication. Ongoing work includes implementing 5' leader transcription, parameter optimization, and longer simulation times to improve predictive accuracy.

Together, these contributions showcase the power of integrated infrastructure and computation in enabling research across virology, medical imaging, and experimental physics.

68. Lipid Remodelling in Extracellular Vesicles from β -Cells under Hyperglycemic Stress - Multimodal Mass Spectrometry Approach

Magdalena Skalska^{1,2}, Martyna Durak-Kozica^{1,2}, Weronika Hewelt-Belka³; Michał Młynarczyk³, Ewa Stepień^{1,2}

¹*Faculty of Physics, Astronomy and Applied Computer Science, Jagiellonian University, Cracow, Poland*

²*Centre for Theranostics, Jagiellonian University, Cracow, Poland*

³*Department of Analytical Chemistry, Chemical Faculty, Gdansk University of Technology, Gdansk, Poland*

Extracellular vesicles (EVs) carry lipid cargo that reflects the metabolic state of their parent cells. We examined the lipid composition of EVs released by pancreatic β -cells under normo and hyperglycaemic conditions. To gain both structural and spatial information, we combined two mass spectrometry methods: high-resolution reversed-phase liquid chromatography with quadrupole time-of-flight mass spectrometry (RP-LC-Q-TOF-MS) and time-of-flight secondary ion mass spectrometry (ToF-SIMS). The study explores how glucose-induced stress modulates the EV lipidome.

Pancreatic β -cells were maintained in normoglycemic medium containing 11 mM (control) and 35 mM (hyperglycaemic) glucose. EVs were isolated using filtration dialysis and ultracentrifugation. Lipids were analysed with RP-LC-Q-TOF-MS following organic extraction, and in semi-native form using label-free ToF-SIMS. The latter enabled spatial imaging of lipid fragments at submicron resolution. Differences in lipid profiles were assessed across conditions and EV subtypes using multivariate analysis. Due to variations in particle numbers, we compared the relative amounts of lipid species within specific lipid classes during the RP-LC-Q-TOF-MS analysis. We focused on lysophosphatidylcholines, phosphatidylcholines, and alkylphosphatidylcholines. Statistically significant differences were observed between groups cultured under varying glucose conditions, particularly between normal glucose levels and an 11 mM glucose concentration in the ectosome group. Additionally, we noted several differences in the content of individual lipids within these classes. These findings were compared with data from ToF-SIMS analysis, which showed significant differences in peak intensities for specific lipids across different populations of EVs and under varying conditions.

The combination of MS/MS and ToF-SIMS provides a powerful approach to lipidomics, especially in analyzing EVs. This integrates precise lipid quantification with spatial imaging, offering valuable insights into lipidomes. It is particularly useful for studying EVs, which carry lipid cargo reflecting their cellular origin and function. By examining both lipid composition and localization researchers gain a deeper understanding of EV biology.

Acknowledgements:

The research was financed by the Polish agency National Science Center as part of two OPUS projects for E.S.: 2022/45/B/NZ7/01430 and 2019/33/B/NZ3/01004 and by WFAIS-Young Laboratories 2024-2 as part of the Excellence – Research University” program at the Jagiellonian University in Kraków.



69. Studies of the absorption parameter 3/2 in positronium decays

Magdalena Skurzok^{1,2}, Kamila Kasperska^{1,2}, Pawel Moskal^{1,2}

¹Faculty of Physics, Astronomy and Applied Computer Science, Jagiellonian University, Cracow, Poland

²Centre for Theranostics, Jagiellonian University, Cracow, Poland

During Positron Emission Tomography (PET), as much as 40% of annihilations happen through the formation of positronium inside the patient's body. Its properties, such as the fraction of positronium annihilations into three photons (3/2), are highly influenced by the tissue's submolecular architecture. This has led to the development of a novel PET imaging techniques - positronium imaging - which provide additional insights into the imaged tissue. Conventional PET devices record only two annihilation photons and cannot assess the properties of positronium. However, the Jagiellonian PET (J-PET) scanner, capable of multiphoton detection, enables three-gamma imaging necessary for determining 3/2 ratio. The aim of this work is to study the absorption of gamma quanta in simplified models approximating the human body, as well as in the XCAT human phantom. For this purpose, toy Monte Carlo (MC) simulations of positronium decays into 2 and 3 and photon absorption in the models were performed and compared with the results obtained with GATE MC simulation tool. Based on the simulations, the dependence of absorption probability of photons in the phantoms on the location of the decay point is determined. As a result of this research, we present absorption maps of para- and ortho-positronium decays, required for data correction.



70. Proton-induced nuclear reactions in the hadrontherapy energy range

Izabela Skwira-Chalot, Tomasz Matulewicz

University of Warsaw, Poland

Proton-induced reactions on tissue not only reduce the beam flux, but also generate radioactivity along the beam trajectory, influencing the effects of proton therapy. Therefore, precise knowledge of cross sections of proton-induced reactions on nuclei the tissue is composed of (oxygen, carbon and nitrogen) is needed for energies below 250 MeV. The production of ^{11}C , ^{13}N and ^{15}O was studied during the past 50 years, but several discrepancies exist even in recent experiments. Furthermore, only few measurements were performed at higher proton energies.

We performed systematic measurements of cross sections using proton beams available at the Institute of Nuclear Physics (Kraków). The experimental set-up, made of 3 pairs of LaBr₃:Ce detectors, was developed at the University of Warsaw. It enables the study of ^{11}C decays from up to 16 simultaneously irradiated targets. Elementary targets (C, BN, SiO₂) and animal tissue samples (liver, heart, bone) were irradiated at AIC-144 cyclotron with protons of energy below 58 MeV [1-6]. The obtained cross sections on C, N and O, are in general agreement with previous measurements, except the ^{11}C production on ^{16}O target [7]. The activity of soft tissues (liver, heart) are dominated by the ^{15}O decay ($T_{1/2}=2$ min) from (p,d) reaction on abundant oxygen nuclei. The production of ^{13}N ($T_{1/2}=10$ min) is increased significantly at low proton energies, what might be related to the peak of the excitation function of $^{16}\text{O}(p,\alpha)^{13}\text{N}$ reaction around 15 MeV.

The future experimental activities concern (i) completion of measurements on nitrogen at $E \leq 58$ MeV, (ii) verification of $^{16}\text{O}(p,\alpha)^{11}\text{C}$ reaction at $E \leq 58$ MeV, and (iii) measurements at higher proton energies available at CCB.

- [1] P. Sekowski et al., Acta Phys. Pol. A 139, 454, 2021
- [2] P. Sekowski et al., Nucl. Instrum. Meth. A 1040, 167292, 2022
- [3] P. Sekowski et al., AIP Conf. Proc. 2778, 2023
- [4] J. Matulewicz et al., Acta Phys. Pol. B Proc. Suppl. 17, 3A-37, 2024
- [5] J. Matulewicz et al., Eur. Phys. J. A 60, 203, 2024
- [6] I. Skwira-Chalot et al., AIP Conf. Proc. 3054, 040006, 2024
- [7] T. Rodriguez-Gonzalez et al., Radiat. Phys. Chem. 190, 109759, 2022



71. Extracellular Vesicles and How to Find Them

Maciej Słotwiński^{1,2}

¹Faculty of Physics, Astronomy and Applied Computer Science, Jagiellonian University, Cracow, Poland

²Centre for Theranostics, Jagiellonian University, Cracow, Poland

Extracellular vesicles (EVs) are a vital part of extracellular communication and transport systems in one's body. They carry various cellular components, such as proteins, mRNAs, miRNAs, DNA, and lipids. Because of their native function in the body, there is a major potential for them to be used in anticancer therapies. However, before that, the most important thing is to get to know them and their behavior as well as possible. For this, various methods could be employed. In this research, an emphasis was put onto quantitative and preliminary qualitative analysis of extracellular vesicles. Two parallel cell cultures with 4 biological repetitions each, were performed. Different glucose concentrations to check how hyperglycemic conditions influence extracellular composition and their production were used. Methods such as ATR-IR, NTA, ToF-SIMS and Cryo TEM were employed and evaluated for vesicle research. Following parameters were measured using ATR-IR and analysed: SFA/UFA ratio, lipid to protein ratio, acyl chain length. Parameters mentioned above, showed no significant difference between both cell culture conditions. For size distribution a comparison of NTA and Cryo TEM was performed. Cells in normoglycemic conditions produced about 100x more EVs and in such conditions exosomes possessed around twice as much cholesterol.



72. Theoretical untangling of photon entanglement detection in positronium annihilation processes

Tomasz Sowinski

Institute of Physics, Polish Academy of Sciences, Warsaw, Poland

When para-positronium annihilation occurs, two photons with exactly the same energy and mutually perpendicular, quantum-mechanically entangled polarizations are emitted in opposite directions. However, experimental confirmation of this effect is not straightforward, because direct detection of the polarization for high-energy gamma photons is not technologically possible. The recent beautiful experiment [1] investigating the angular correlations of Comptonscattered photons originating from annihilation has actually brought us much closer to experimental confirmation that the emitted photons are most probably entangled. During the lecture, however, I will show that it is still possible that the detected angular correlations come from classical correlations. Based on the methods of quantum metrology, I will also propose a direction in which the experiment should be modified to confirm the quantum entanglement of such photons.

[1] P. Moskal et al., Sci. Adv. 11, eads3046, 2025



73. EVs as a non-invasive approach to diagnose and monitor metabolic diseases

E.Ł. Stępień ^{1,2}

¹*Faculty of Physics, Astronomy and Applied Computer Science, Jagiellonian University, Cracow, Poland*

²*Centre for Theranostics, Jagiellonian University, Cracow, Poland*

The molecular composition of EVs is very complex, with lipid and protein components dominating [1-3]. Although it is known that they are composed of the same macromolecules as the cells from which they originate, we have observed differences between the proportion of macromolecules in different subpopulations of EVs and cells [4]. The proportions and share of individual protein and lipid metabolites also change depending on the metabolic state of the cells from which the individual EV fractions originate [1,5]. One of the main factors influencing their molecular composition is hyperglycemia, which we have observed in an in vitro model of pancreatic beta cells and in clinical studies in patients with diabetes [5-8]. The presentation will show the results of metabolomic studies of small and large EVs isolated from patients with type 1 and 2 diabetes and from in vitro cultures of beta-pancreatic cells in conditions of mild and high hyperglycemia.

SciMat and qLife Priority Research Area budget under the Strategic Programme Excellence Initiative at the Jagiellonian University; 2019/33/B/NZ3/01004 and 2022/45/B/NZ7/01430 Narodowe Centrum Nauki

- [1] M. E. Marzec, C. Rząca, P. Moskal, and E. Ł. Stępień, *Biochem. Biophys. Res. Commun.*, vol. 622, pp. 30–36, 2022.
- [2] B. Zapata et al., *Pharm. Res.*, vol. 40, no. 4, pp. 817–832, 2023.
- [3] J. Kasprzyk-Pochopień et al., *Molecules*, vol. 30, no. 6, p. 1384, 2025.
- [4] M. Roman et al., *Nanomedicine*, vol. 17, pp. 137–149, 2019.
- [5] M. E. Skalska, M. Durak-Kozica, and E. Ł. Stępień, *Talanta*, published online Jul. 15, 2025.
- [6] E. Ł. Stępień et al., *Theranostics*, vol. 8, no. 14, pp. 3874–3890, 2018.
- [7] A. Kamińska et al., *Nanomedicine*, vol. 39, p. 102468, 2022.



74. A Geant 4 simulation of the positronium target cloud in the GBAR experiment

Karol Szymczyk

National Centre for Nuclear Research, Poland

The Gravitational Behaviour of Antihydrogen at Rest (GBAR) experiment at CERN aims to explore a fundamental property of neutral antihydrogen, the gravitational interaction. The Antiproton Decelerator and ELENA ring complex at CERN produces a beam of 100 keV antiprotons. An antiproton from this beam is merged with positronium cloud [1,2] to form a cold, positively charged antihydrogen ion, suitable for free-fall measurements. Antihydrogen ions are created via two successive reactions involving a dense positronium (Ps) cloud:

$p + \text{Ps} \rightarrow \text{H} + e$ followed by $\text{H} + \text{Ps} \rightarrow \text{H}^+ + e$

The Ps cloud is generated by reacting positrons with a nanoporous SiO converter. The cloud density plays a key role in the efficient H and H⁺ production.

A dedicated Monte Carlo simulation has been developed in Geant4 specifically for the GBAR experiment, including details of the generation and propagation of the positronium cloud inside the reaction cavity. An antiproton beam has been included, enabling in-simulation production of antihydrogen atoms directly within the reaction chamber through Ps-p interactions.

Data taken in 2024 should allow determination of the cross section for antihydrogen production in the first reaction at 4 and 6 keV antiproton beam energy. The results should provide a test of theoretical models that predict different values for this cross section.[3]

The poster presents the current status of the simulation, including updated geometry, Ps-H processes, and shows how the simulation of the H formation in the Ps cloud helps in the interpretation of the experimental data.

[1] GBAR Collaboration, Nucl. Instrum. Meth. A 1040, 167263, 2022

[2] GBAR Collaboration, Nucl. Instrum. Meth. A 985, 164657, 2021

[3] GBAR Collaboration, Eur. Phys. J. C 83, 1004, 2023



75. Search for eta'-mesic nuclei with (p,dp) reaction at GSI/FAIR

Yoshiki Tanaka

RIKEN, Japan

We performed missing-mass spectroscopy of the $^{12}\text{C}(p,d)$ reaction near the η' -meson emission threshold to search for η' -mesic nuclei—bound states of the η' meson and a nucleus—in order to study in-medium η' -meson properties, which are closely related to the axial U(1) anomaly and chiral symmetry breaking in QCD. The experiment was conducted using a recently developed setup that integrates the WASA central detector into the fragment separator FRS at GSI. The missing mass of the reaction was measured using the FRS operated as a high-resolution forward spectrometer. In addition, the large-acceptance WASA detector was used in coincidence to tag particles, particularly high-momentum protons, emitted from the decay of η' -mesic nuclei. This tagging suppressed background contributions in the (p,d) reaction and thus enhanced the experimental sensitivity to η' -mesic nucleus formation. In this talk, we will introduce the experiment and present preliminary results obtained from the data analysis.



76. Towards Charge conjugation symmetry test in Electromagnetic Interaction using J-PET

Pooja Tanty^{1,2}, Elena Perez del Rio^{1,2}, Pawel Moskal^{1,2}, and for the J-PET Collaboration

¹*Faculty of Physics, Astronomy, and Applied Computer Science, Jagiellonian University, Cracow, Poland,*

²*Centre for Theranostics, Jagiellonian University, Cracow, Poland*

Charge conjugation symmetry (C symmetry) still remains a fundamental symmetry in the realm of physics. It is well-known to be maximally violated in weak interactions. However, its validity is yet to be tested in Electromagnetic (EM) and Strong interactions. With the aim to test this symmetry in EM interactions, the forbidden decay channel of the triplet Positronium state – the ortho-Positronium (oPs) shall be explored. The C symmetry forbids this state from decay into anything other than an odd number of photons; henceforth a search for four-photon decay extends the feasibility of testing the C symmetry in EM interaction using a J-PET detector. Furthermore, the bosonic nature of photons hints at a distinct configuration in the event of a C-symmetry violation. Known for its outstanding timing (~ 250 ps) and angular ($\sim 1^\circ$) resolutions, J-PET offers a viable and substantial platform to perform this symmetry test.

J-PET series of detectors has previously established its credibility in the tests of discrete symmetries, further supporting the feasibility of the aforementioned test. In this presentation, the motivation behind the study, the theoretical assumptions, and recent advancements in the test of C symmetry using J-PET shall be discussed.

We acknowledge support from the National Science Centre of Poland through Grants No. 2019/35/B/ST2/03562, 2020/38/E/ST2/00112, and the SciMat and qLife Priority Research Area budget under the auspices of the program Excellence Initiative-Research University at Jagiellonian University.

[1] P. Moskal et al., Nat. Commun., vol. 12, p. 5658, 2021.

[2] P. Moskal et al., Nat. Commun., vol. 15, p. 78, 2024.

[3] P. Moskal et al., Sci. Adv., vol. 7, p. eabh4394, 2021.

[4] P. Moskal et al., Sci. Adv., vol. 10, p. eadp2840, 2024.

[5] P. Moskal et al., Sci. Adv., vol. 11, p. eads3046, 2025.

[6] Mani and Rich, Phys. Rev. D, vol. 4, p. 122, 1970.



77. A Feasibility Study of Using Detector-Scattered Photons for Attenuation Map Generation in J-PET Scanner

Satyam Tiwari^{1,2}, Sushil Sharma^{1,2} and Pawel Moskal^{1,2} on behalf of the J-PET collaboration

¹*Faculty of Physics, Astronomy, and Applied Computer Science, Jagiellonian University, Cracow, Poland,*

²*Centre for Theranostics, Jagiellonian University, Cracow, Poland*

Quantitative accuracy in Positron Emission Tomography (PET) depends on reliable attenuation correction (AC) methods [1,2]. The clinical standard for AC in PET imaging remains computed tomography (CT). However, this approach increases patient radiation dose and imaging expenses. In recent years, several CT-less attenuation correction methodologies have been proposed to eliminate the need for CT scans [3,4,5]. In this work, we present a feasibility study for a CT-less AC approach that utilizes photons undergoing Compton scattering within the PET detector—data typically discarded in conventional analyses. This method is especially well-suited to the J-PET scanner [6], which is built from long plastic scintillators that inherently produce a significant number of detectable scattered photons [7,8].

We performed simulations using the GEANT4 Application for Tomographic Emission (GATE) [9] by modeling a modular J-PET scanner [10] with phantoms having varying attenuation profiles. We then analyzed the Lines of Response (LORs) formed between the first interaction at the detector and the subsequent detection of the scattered photon after it passes through the phantom and reaches the detector on the opposite side. An algorithm was developed to extract attenuation properties from these unique LORs, thereby generating coarse attenuation maps. Our initial findings show that these LORs contain spatial information about the phantom's attenuation distribution, enabling the distinction between soft tissue and bone-equivalent regions. These results demonstrate that detector-scattered photons can serve as an intrinsic data source for generating attenuation maps.

In this presentation, we will discuss the methodology and results of this feasibility study.

[1] P. E. Kinahan et al., *Med. Phys.*, vol. 25, pp. 2046–2053, 1998.

[2] H. Zaidi et al., *J. Nucl. Med.*, vol. 44, pp. 291–315, 2003.

[3] Y. Berker et al., *Med. Phys.*, vol. 43, pp. 807–832, 2016.

[4] H. Arabi et al., Deep learning-guided estimation of attenuation correction factors from time-of-flight PET emission data

[5] M. Rezaei, Z. A. K. Zadeh, A. R. Rastghalam, M. H. Doulatatabadi, and M. Shamsaei, *J. Biomed. Phys. Eng.*, vol. 10, no. 2, pp. 249–264, 2020.

[6] P. Moskal et al., *Bio-Algorithms Med-Syst.*, vol. 7, no. 2, 2011.

[7] S. Niedzwiecki et al., *Acta Phys. Pol. B*, vol. 48, p. 1567, 2017.

- [8] P. Kowalski et al., *Acta Phys. Pol. B*, vol. 47, no. 2, 2016.
- [9] S. Jan et al., *Phys. Med. Biol.*, vol. 49, no. 19, pp. 4543–4561, 2004.
- [10] P. Moskal et al., *Phys. Med. Biol.*, vol. 66, no. 17, 2021.



78. Development of a millifluidic platform for slow positron beam studies of biological samples

M. Vicini^{1*}, M. De Marchi¹, C. Martinelli¹, M. Laganà², P. Folegati³, C. Giordano¹, M.T. Raimondi¹, C. Conci¹, R. Ferragut^{3,4}

¹*Department of Chemistry, Materials and Chemical Engineering “G. Natta”, Politecnico di Milano, Milan, Italy,*

²*Gemma Advanced Prototypes, 20236 Erba (CO), Italy*

³*Department of Physics, Politecnico di Milano, Milan, Italy*

⁴*INFN, Sezione di Milano, Milano, Italy*

Positron annihilation spectroscopy (PAS) gained increased attention in recent years for its ability to probe structural and chemical variations in cells and tissues. For instance, the technique successfully identified the presence of skin cancer or hypoxia in spheroids [1,2]. Because of this capability, added to the non-destructive nature of the method, PAS has the potential to improve the informative content of positron emission tomography (PET) acquisitions [3]. However, the quasi-totality of PAS studies is currently performed with a standard ²²Na drop-casted source and/or fixed tissues or cells. This means that it is still unknown how a particular cell type or tissue layer affects lifetime and energy spectra of positrons. Here, we present a system enabling the coupling of living biological matter to a variable energy positron beam, enabling precise control of implantation depth inside the sample.

The system prototypes consist of two 3D-printed parts: an upper one with a coverslip glass for optical access and a bottom one with a 2.5×2.5 mm square silicon nitride (Si₃N₄) window with a thickness of 200 nm. The window works as an interface between the high vacuum chamber of the positron beam and the biological sample at atmospheric pressure inside the culture chamber. In addition, a millifluidic circuit ensures the viability of cells throughout the acquisition. We performed preliminary PAS measurements on confluent monolayers of endothelial cells (H5V and bend.3), cultured directly inside the prototype, as a model of microcirculation capillaries.

In conclusion, we developed an innovative, compact, low-cost system for the measurements of complex biological systems with a variable energy positron beam. The prototypes resulted in being watertight and reliable when coupled to the vacuum chamber of the positron beam of our laboratory. The perfusion system provided optimal cell culture conditions for cell viability, as confirmed by epifluorescence and microscopy images acquired through the optical window. In addition, we tested the system using a high vacuum chamber and performed preliminary PAS measurements on cells. This technological advancement is a step forward in the understanding of the interaction of antimatter with biological systems at the nanoscale, important for the potential future application of the technique for diagnostic purposes.

Acknowledgments

ERC, project BEACONSANDEGG, G.A. 101053122; MUR, project INFLAMMATRON, D43C23002400008.

[1] Y. C. Jean et al., "Applied Surface Science," vol. 252, no. 9, pp. 3166–3171, 2006.

[2] H. Karimi et al., "Scientific Reports," vol. 13, no. 1, 2023.

[3] P. Moskal et al., "Science Advances," vol. 10, no. 37, 2024.